
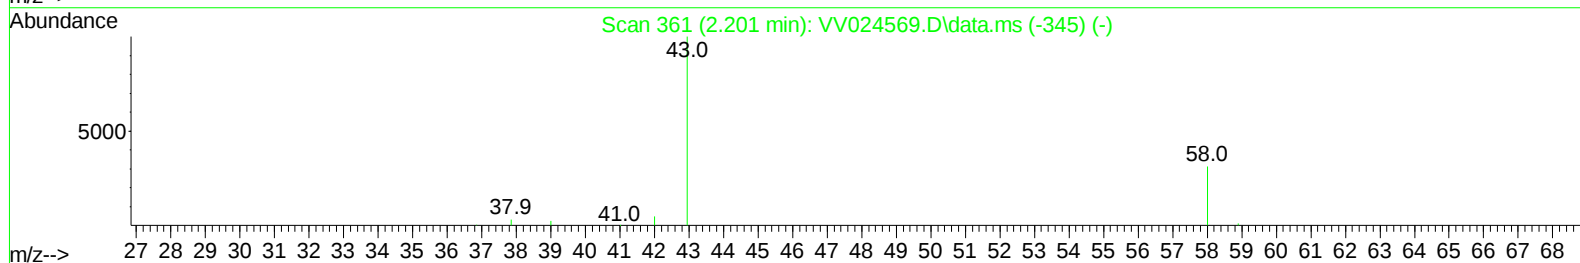
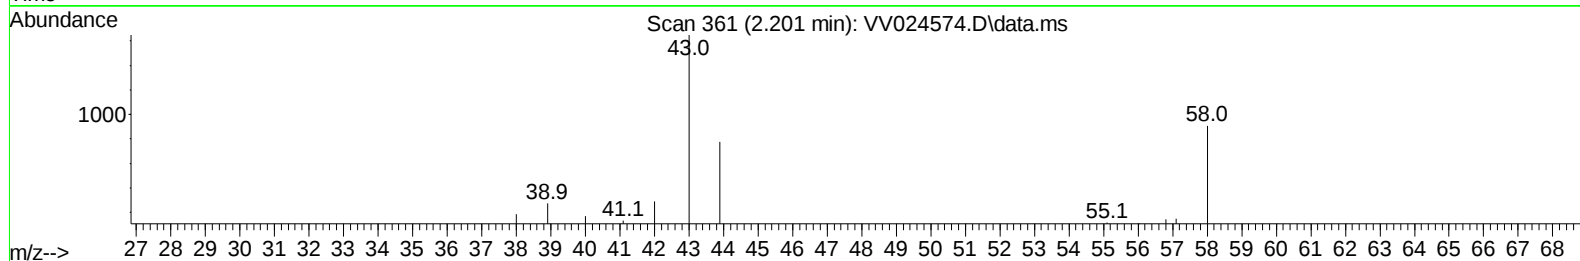


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021022\
Data File : VV024574.D
Acq On : 10 Feb 2022 17:39
Operator : SY/MD
Sample : N1476-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Feb 11 04:52:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 11 04:51:03 2022
Response via : Initial Calibration

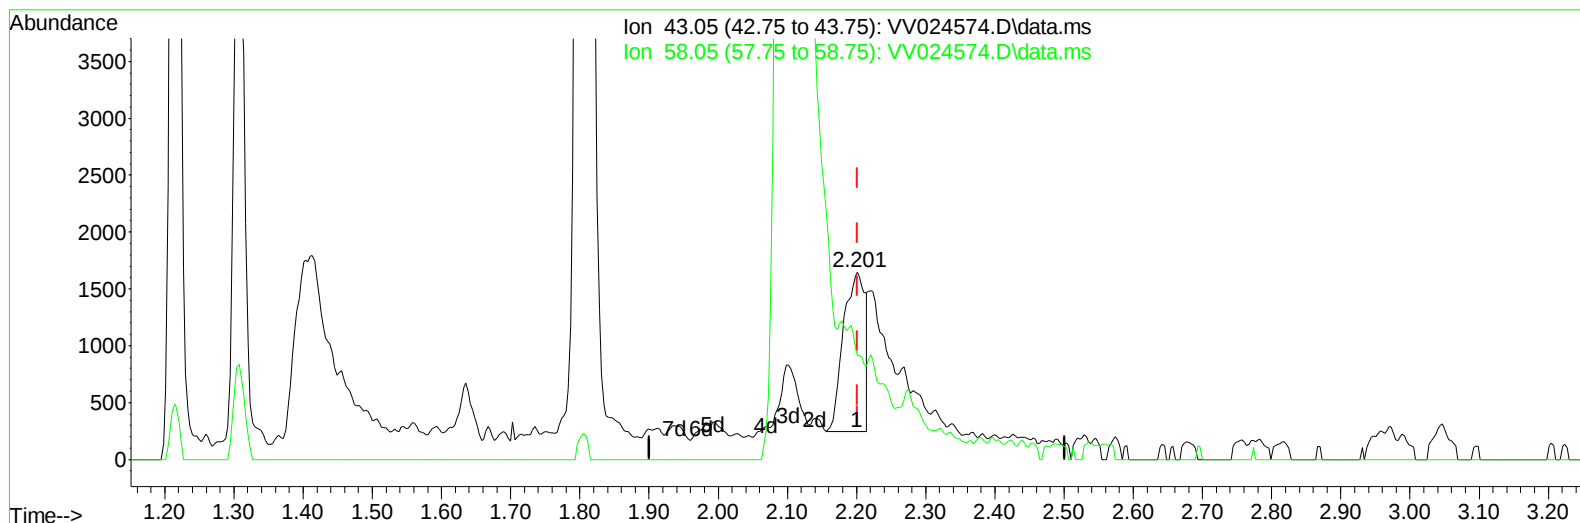

TIC: VV024574.D\data.ms

(13) Acetone (T)




2.201min (-0.000) 1.96 ug/L

response 3052

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	0.00
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021022\
Data File : VV024574.D
Acq On : 10 Feb 2022 17:39
Operator : SY/MD
Sample : N1476-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Feb 11 04:52:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 11 04:51:03 2022
Response via : Initial Calibration

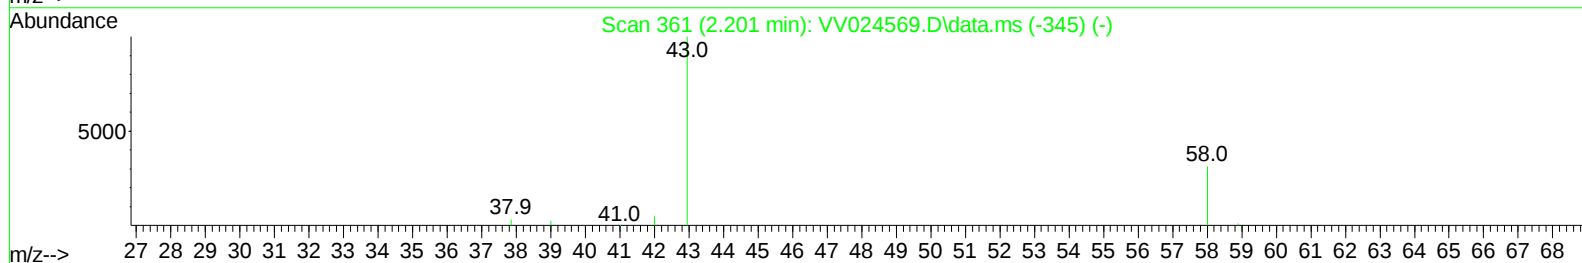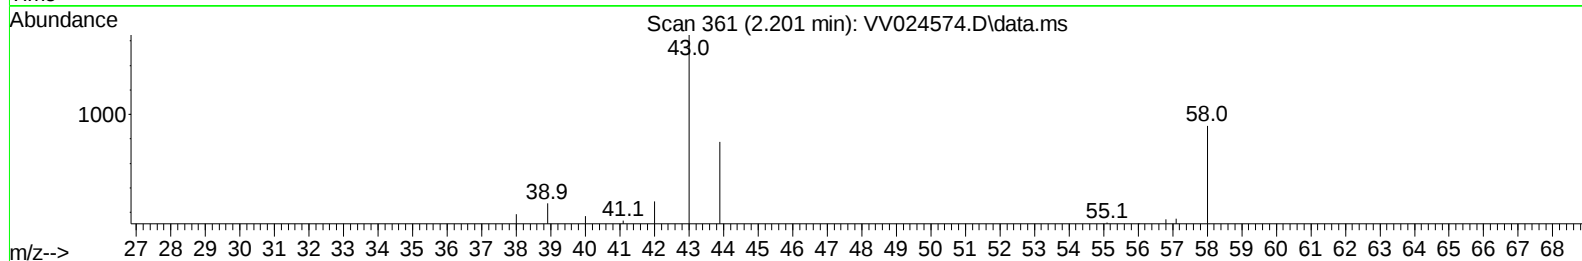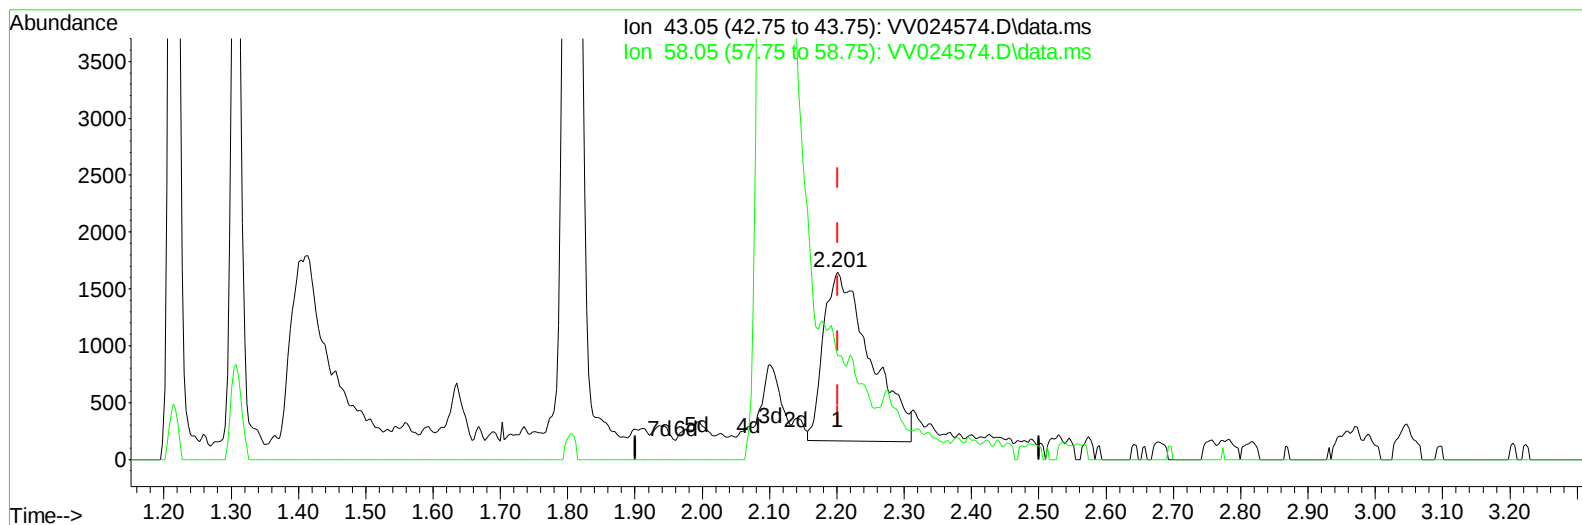

TIC: VV024574.D\data.ms

(13) Acetone (T)

2.201min (-0.000) 4.61 ug/L m

response 7178

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	0.00
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021022\
 Data File : VV024574.D
 Acq On : 10 Feb 2022 17:39
 Operator : SY/MD
 Sample : N1476-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Quant Time: Feb 11 04:52:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 11 04:51:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	141664	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	139543	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	71373	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	49682	4.184	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	83.600%	
7) Chloroethane-d5	1.568	69	44792	4.462	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	89.200%	
11) 1,1-Dichloroethene-d2	2.108	63	80305	3.092	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	61.800%	
20) 2-Butanone-d5	3.908	46	86845	44.055	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	88.100%	
24) Chloroform-d	4.349	84	96704	4.627	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	92.600%	
26) 1,2-Dichloroethane-d4	5.034	65	45320	4.779	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	95.600%	
32) Benzene-d6	5.050	84	190965	4.823	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	96.400%	
36) 1,2-Dichloropropane-d6	6.069	67	58666	4.764	ug/L	0.00
41) Toluene-d8	7.313	98	177151	4.797	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	96.000%	
43) trans-1,3-Dichloroprop...	7.625	79	22809	4.587	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	91.800%	
46) 2-Hexanone-d5	8.088	63	86717	49.495	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	99.000%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	34065	4.646	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	93.000%	
66) 1,2-Dichlorobenzene-d4	11.622	152	53793	4.676	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	93.600%	
Target Compounds						
					Qvalue	
13) Acetone	2.201	43	7178m	4.614	ug/L	
25) Chloroform	4.381	83	10352	0.397	ug/L	91
47) Tetrachloroethene	7.973	164	129388	13.005	ug/L	91
53) m,p-xylene	9.146	106	1108	0.044	ug/L	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021022\
Data File : VV024574.D
Acq On : 10 Feb 2022 17:39
Operator : SY/MD
Sample : N1476-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Feb 11 04:52:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 11 04:51:03 2022
Response via : Initial Calibration

