
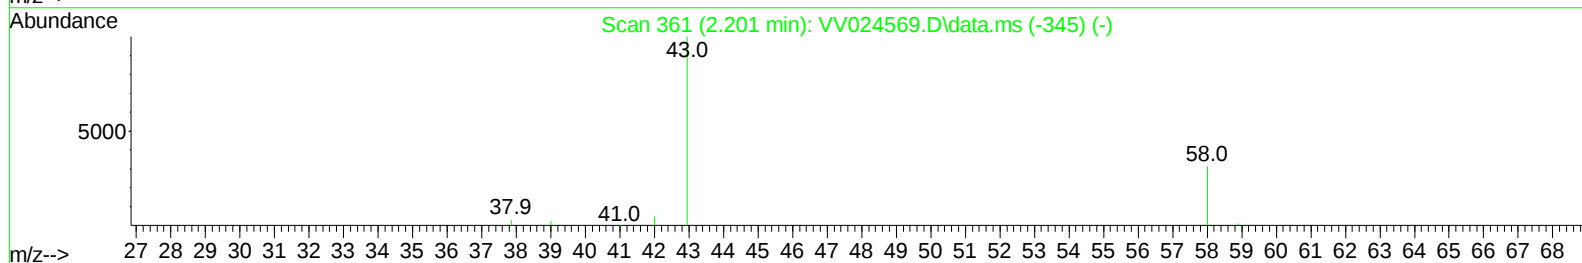
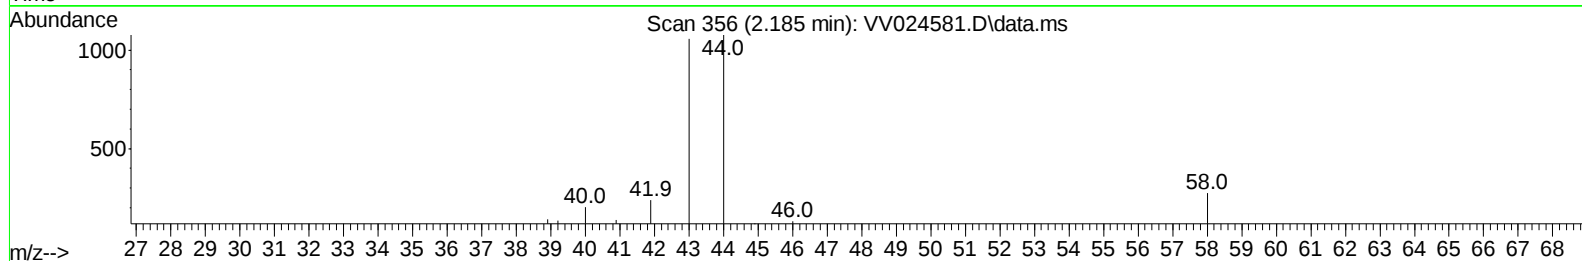


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021022\
Data File : VV024581.D
Acq On : 10 Feb 2022 20:23
Operator : SY/MD
Sample : N1475-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Feb 11 04:54:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 11 04:51:03 2022
Response via : Initial Calibration

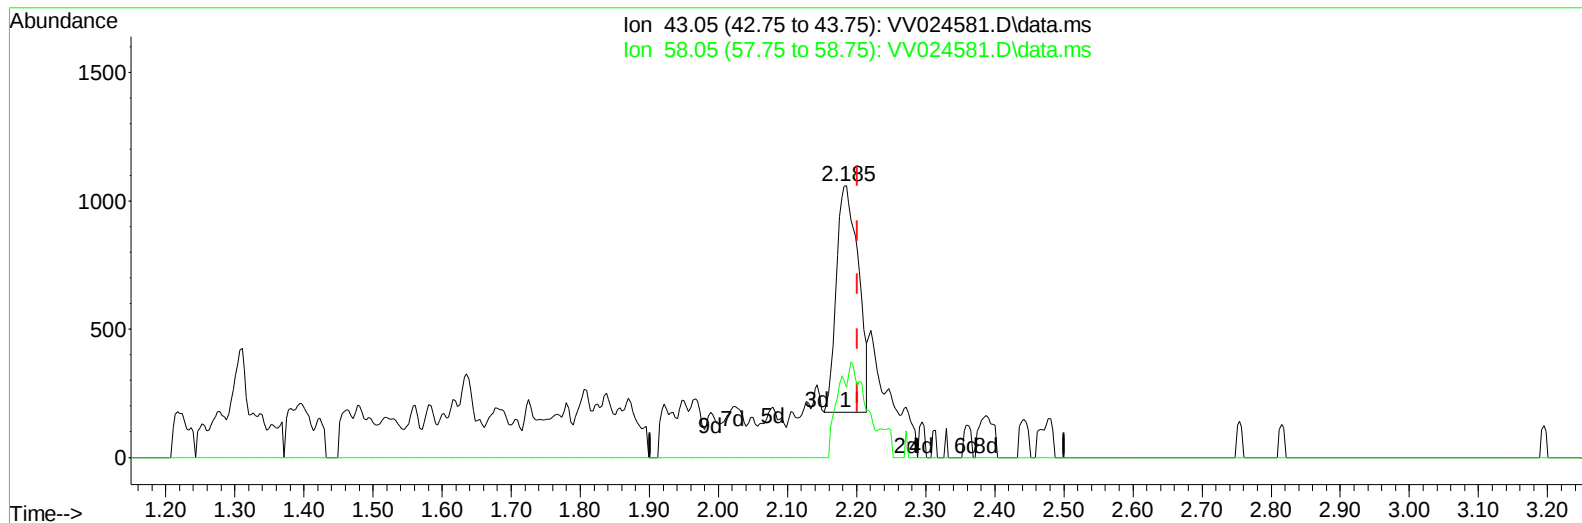

TIC: VV024581.D\data.ms

(13) Acetone (T)




2.185min (-0.016) 1.40 ug/L

response 1941

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	23.03
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021022\
Data File : VV024581.D
Acq On : 10 Feb 2022 20:23
Operator : SY/MD
Sample : N1475-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Feb 11 04:54:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 11 04:51:03 2022
Response via : Initial Calibration

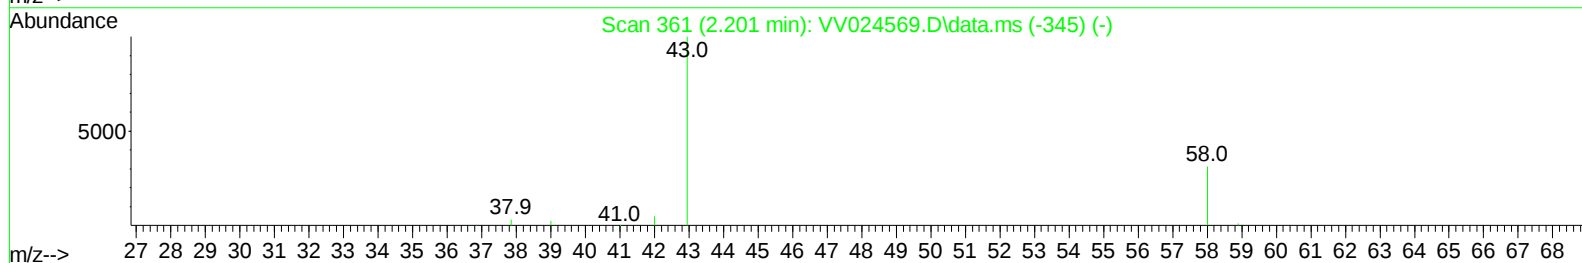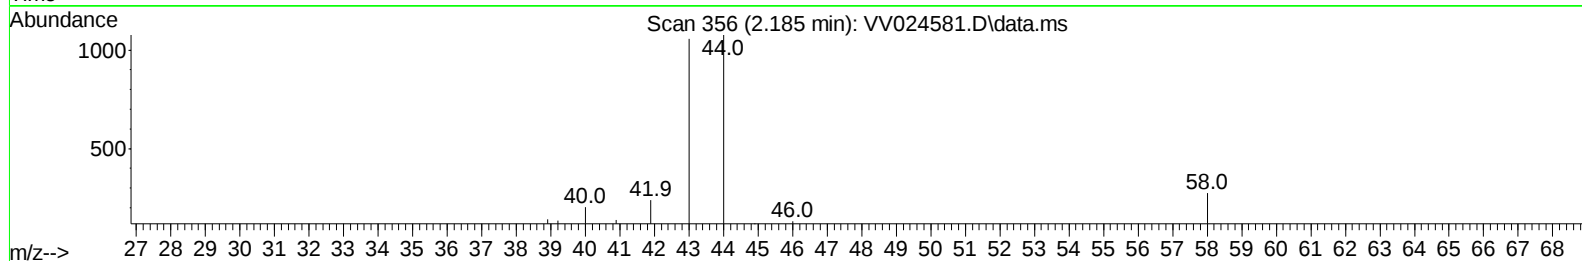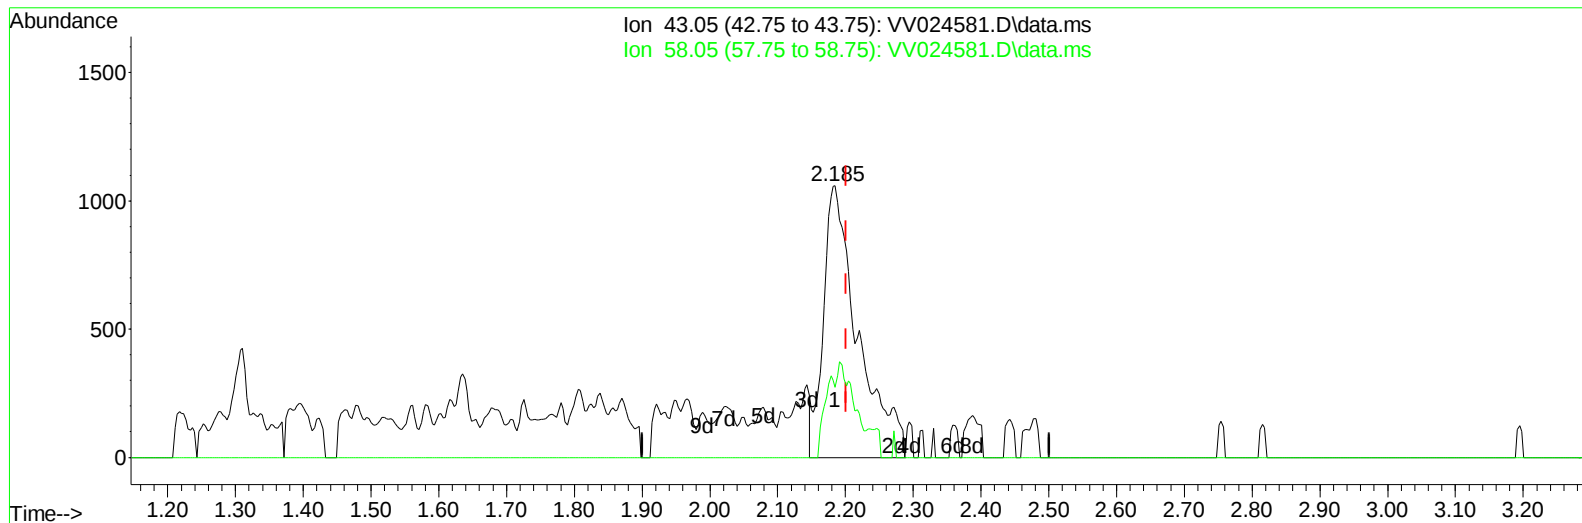

TIC: VV024581.D\data.ms

(13) Acetone (T)

2.185min (-0.016) 2.70 ug/L m

response 3727

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	11.99
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021022\
 Data File : VV024581.D
 Acq On : 10 Feb 2022 20:23
 Operator : SY/MD
 Sample : N1475-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Feb 11 04:54:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 11 04:51:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	125915	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	124294	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	62133	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	41720	3.953	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	79.000%	
7) Chloroethane-d5	1.571	69	39579	4.436	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	88.800%	
11) 1,1-Dichloroethene-d2	2.111	63	68613	2.972	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	59.400%#	
20) 2-Butanone-d5	3.899	46	91971	52.490	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	104.980%	
24) Chloroform-d	4.352	84	86938	4.680	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	93.600%	
26) 1,2-Dichloroethane-d4	5.034	65	42472	5.039	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	100.800%	
32) Benzene-d6	5.053	84	176165	4.995	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	100.000%	
36) 1,2-Dichloropropane-d6	6.069	67	54589	4.977	ug/L	0.00
41) Toluene-d8	7.317	98	158813	4.828	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	96.600%	
43) trans-1,3-Dichloroprop...	7.625	79	20100	4.538	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	90.800%	
46) 2-Hexanone-d5	8.088	63	79260	50.789	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	101.580%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	30439	4.661	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	93.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152	50227	5.015	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	100.200%	
Target Compounds						
					Qvalue	
25) Chloroform	4.384	83	4784	0.207	ug/L	98
42) Toluene	7.387	91	2285161	43.243	ug/L	99
52) Ethylbenzene	9.018	91	6383	0.109	ug/L	90
53) m,p-xylene	9.143	106	7767	0.349	ug/L	95
54) o-xylene	9.545	106	2489	0.116	ug/L	83
55) Styrene	9.571	104	3727	0.106	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021022\
Data File : VV024581.D
Acq On : 10 Feb 2022 20:23
Operator : SY/MD
Sample : N1475-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Feb 11 04:54:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 11 04:51:03 2022
Response via : Initial Calibration

