




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021022\
 Data File : VV024587.D
 Acq On : 10 Feb 2022 22:43
 Operator : SY/MD
 Sample : N1475-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4M09

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 02/15/2022
 Supervised By :Semsettin Yesilyurt 02/17/2022

Quant Time: Feb 11 23:59:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 11 23:54:44 2022
 Response via : Initial Calibration

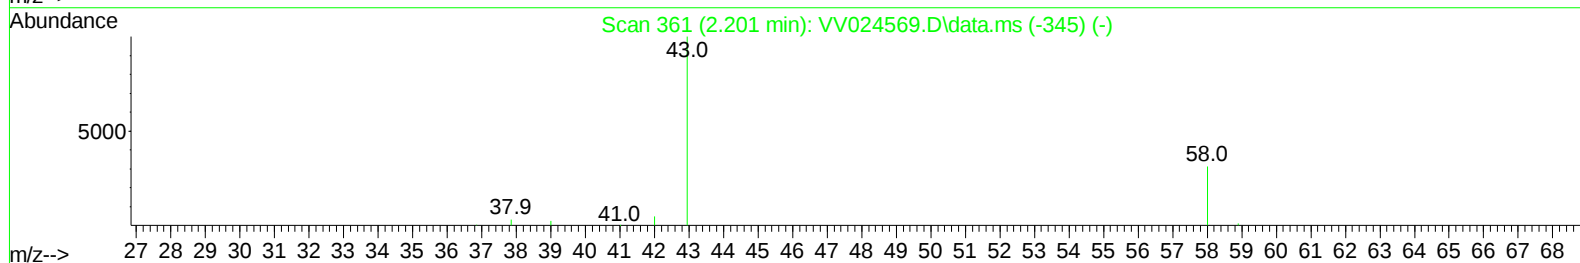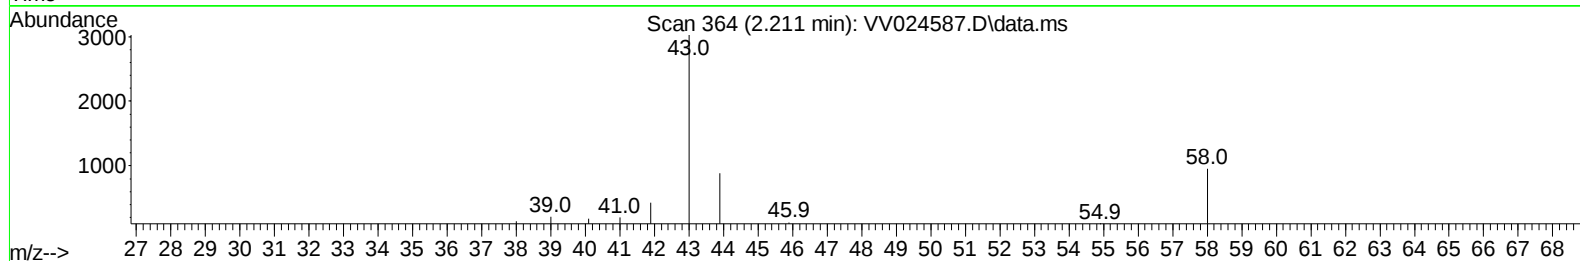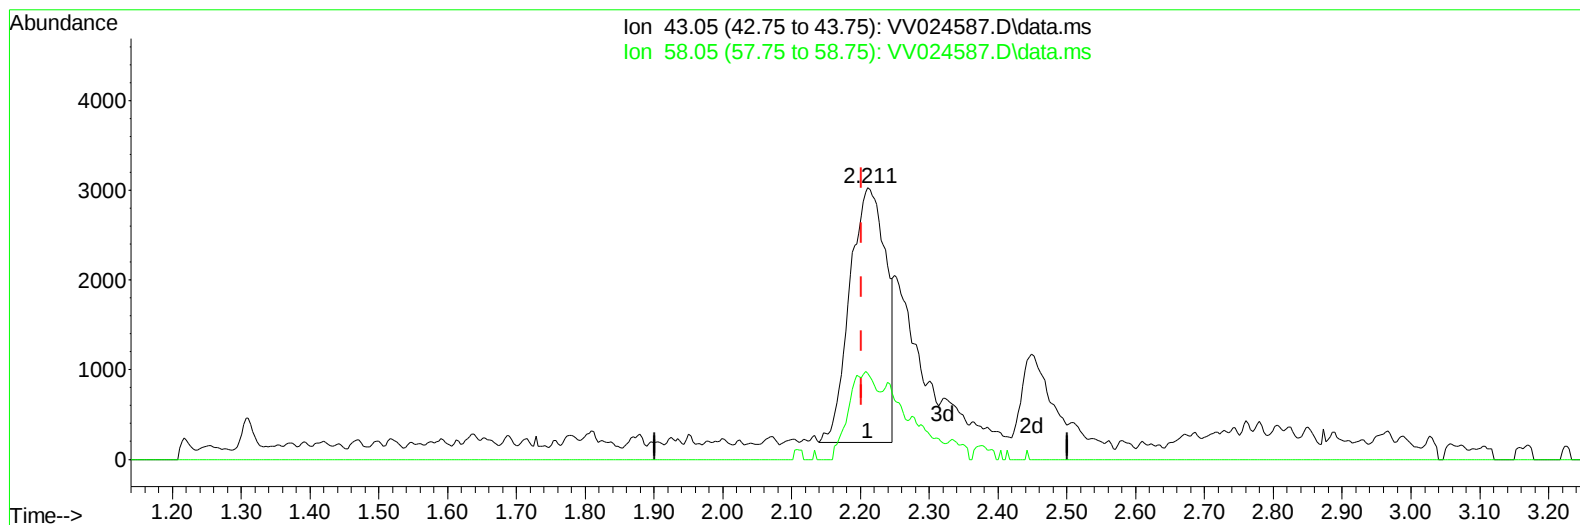

TIC: VV024587.D\data.ms

(13) Acetone (T)

2.211min (+ 0.009) 7.89 ug/L

response 10378

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	26.43
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021022\
Data File : VV024587.D
Acq On : 10 Feb 2022 22:43
Operator : SY/MD
Sample : N1475-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M09

Manual IntegrationsAPPROVED

Quant Time: Feb 11 23:59:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 11 23:54:44 2022
Response via : Initial Calibration

Reviewed By :John Carlone 02/15/2022
Supervised By :Semsettin Yesilyurt 02/17/2022

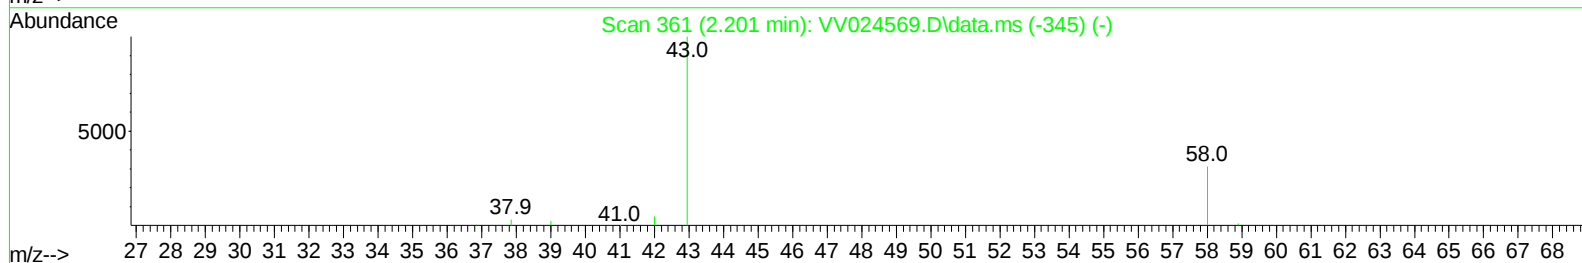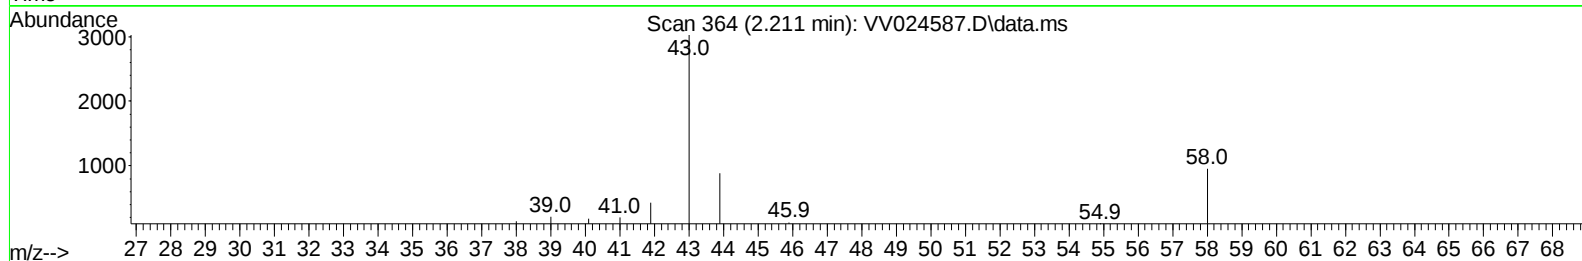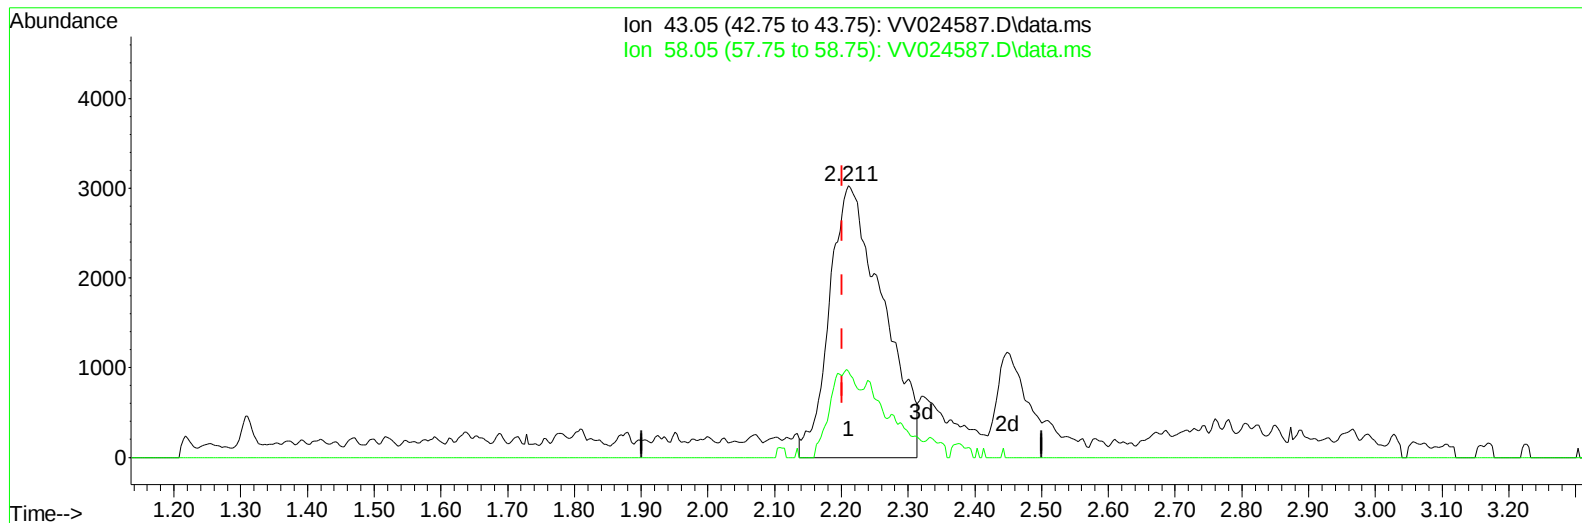

TIC: VV024587.D\data.ms

(13) Acetone (T)

2.211min (+ 0.009) 12.74 ug/L m

response 16757

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	16.37
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021022\
 Data File : VV024587.D
 Acq On : 10 Feb 2022 22:43
 Operator : SY/MD
 Sample : N1475-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4M09

Manual IntegrationsAPPROVED

Quant Time: Feb 11 23:59:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 11 23:54:44 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 02/15/2022
 Supervised By :Semsettin Yesilyurt 02/17/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.619	114		119761	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117		118739	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152		59356	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.307	65		40748	4.059	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.200%	
7) Chloroethane-d5	1.571	69		37349	4.401	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.000%	
11) 1,1-Dichloroethene-d2	2.111	63		66601	3.033	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.600%	
20) 2-Butanone-d5	3.921	46		73270	43.966	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	87.940%	
24) Chloroform-d	4.349	84		82102	4.647	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.000%	
26) 1,2-Dichloroethane-d4	5.034	65		39537	4.932	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.600%	
32) Benzene-d6	5.050	84		165268	4.906	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.200%	
36) 1,2-Dichloropropane-d6	6.069	67		50431	4.813	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.200%	
41) Toluene-d8	7.317	98		149713	4.765	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.200%	
43) trans-1,3-Dichloroprop...	7.625	79		18331	4.332	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.600%	
46) 2-Hexanone-d5	8.088	63		68384	45.870	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.740%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84		31179	4.997	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.000%	
66) 1,2-Dichlorobenzene-d4	11.622	152		48357	5.054	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.000%	
Target Compounds							
						Qvalue	
13) Acetone	2.211	43		16757m	12.742	ug/L	
14) Carbon disulfide	2.297	76		52699	1.337	ug/L	99
15) Methyl Acetate	2.449	43		2417	0.643	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021022\
Data File : VV024587.D
Acq On : 10 Feb 2022 22:43
Operator : SY/MD
Sample : N1475-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M09

Manual IntegrationsAPPROVED

Quant Time: Feb 11 23:59:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 11 23:54:44 2022
Response via : Initial Calibration

Reviewed By :John Carlone 02/15/2022
Supervised By :Semsettin Yesilyurt 02/17/2022

