




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021022\
 Data File : VV024588.D
 Acq On : 10 Feb 2022 23:06
 Operator : SY/MD
 Sample : N1475-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4M10

Manual IntegrationsAPPROVED

Quant Time: Feb 11 23:59:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 11 23:54:44 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 02/15/2022
 Supervised By :Semsettin Yesilyurt 02/17/2022

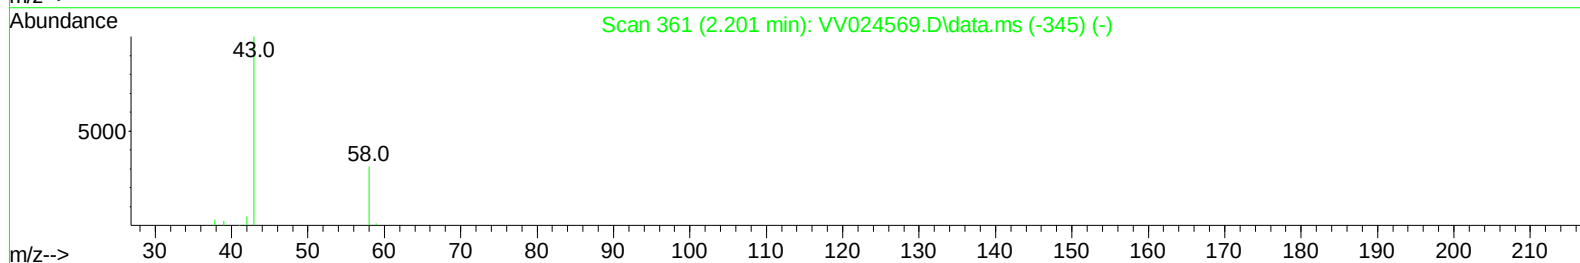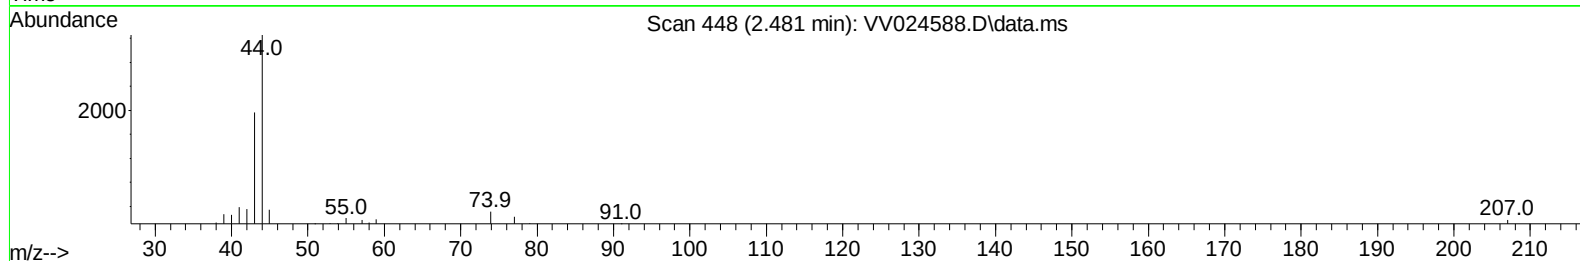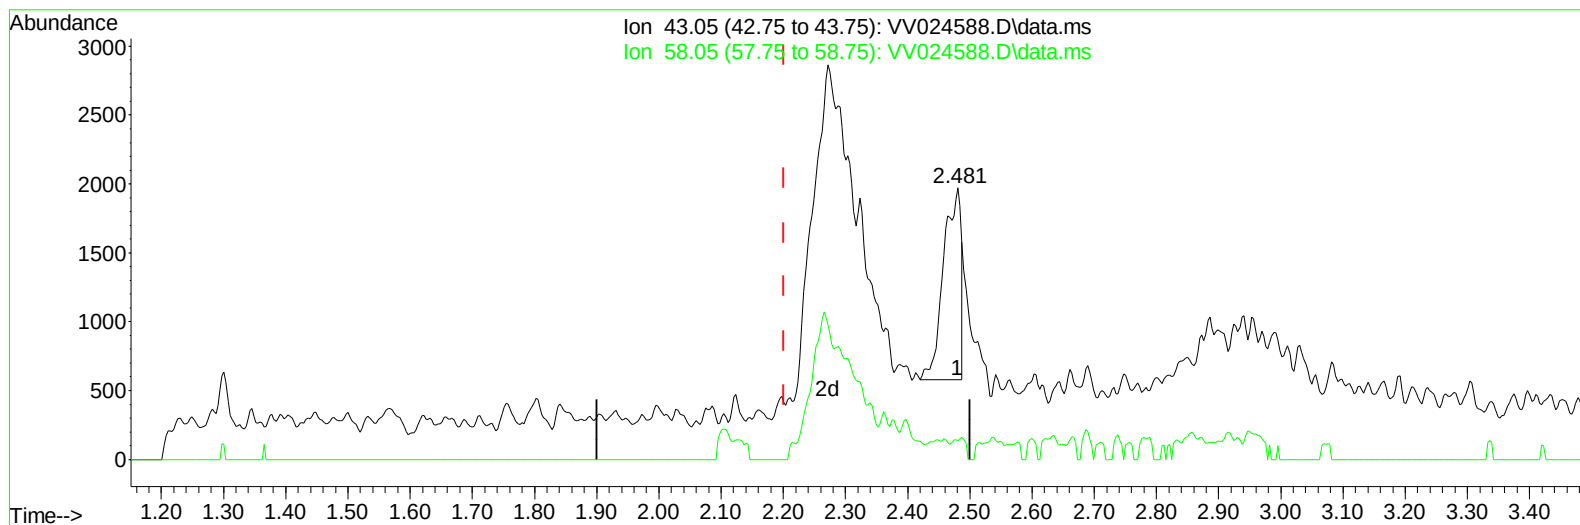

TIC: VV024588.D\data.ms

(13) Acetone (T)

2.481min (+ 0.280) 2.11 ug/L

response 2741

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	6.82
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021022\
Data File : VV024588.D
Acq On : 10 Feb 2022 23:06
Operator : SY/MD
Sample : N1475-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M10

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 02/15/2022
Supervised By :Semsettin Yesilyurt 02/17/2022

Quant Time: Feb 11 23:59:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 11 23:54:44 2022
Response via : Initial Calibration

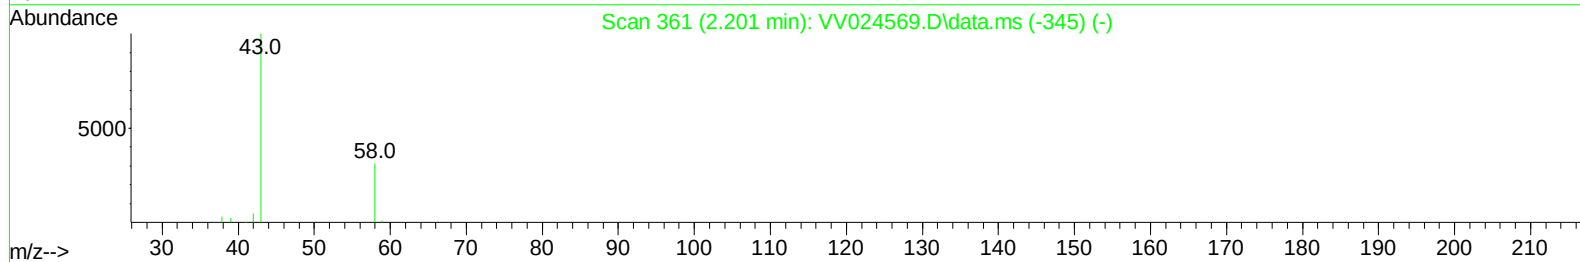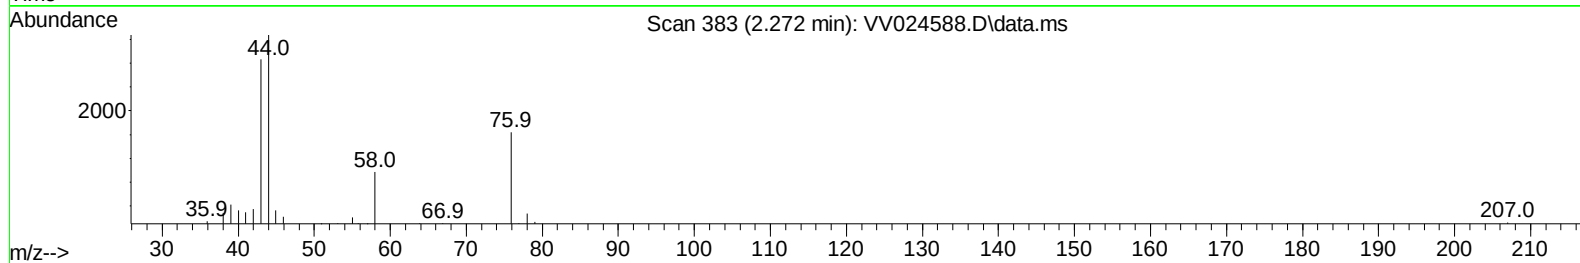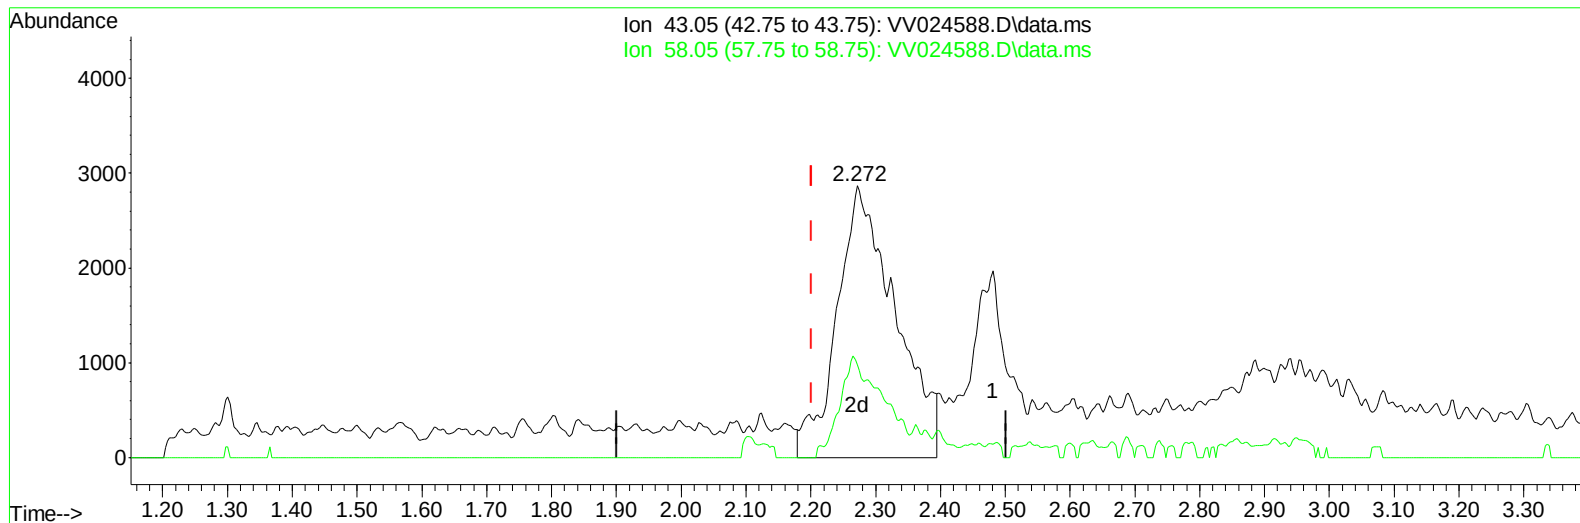

TIC: VV024588.D\data.ms

(13) Acetone (T)

2.272min (+ 0.071) 13.77 ug/L m

response 17887

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	1.05
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021022\
 Data File : VV024588.D
 Acq On : 10 Feb 2022 23:06
 Operator : SY/MD
 Sample : N1475-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4M10

Manual IntegrationsAPPROVED

Quant Time: Feb 11 23:59:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 11 23:54:44 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 02/15/2022
 Supervised By :Semsettin Yesilyurt 02/17/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	118330	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	114498	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	57380	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	49168	4.957	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	99.200%		
7) Chloroethane-d5	1.561	69	43812	5.225	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	104.400%		
11) 1,1-Dichloroethene-d2	2.101	63	70853	3.266	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	65.400%		
20) 2-Butanone-d5	3.979	46	87814	53.331	ug/L	0.07
Spiked Amount 50.000	Range 40 - 130		Recovery =	106.660%		
24) Chloroform-d	4.342	84	82833	4.745	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	94.800%		
26) 1,2-Dichloroethane-d4	5.034	65	38161	4.818	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	96.400%		
32) Benzene-d6	5.043	84	161153	4.961	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	99.200%		
36) 1,2-Dichloropropane-d6	6.069	67	49605	4.909	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	98.200%		
41) Toluene-d8	7.313	98	148111	4.888	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	97.800%		
43) trans-1,3-Dichloroprop...	7.625	79	17081	4.186	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	83.800%		
46) 2-Hexanone-d5	8.101	63	55925	38.902	ug/L	0.01
Spiked Amount 50.000	Range 45 - 130		Recovery =	77.800%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	30200	5.020	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	100.400%		
66) 1,2-Dichlorobenzene-d4	11.622	152	48186	5.210	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	104.200%		
Target Compounds						
					Qvalue	
13) Acetone	2.272	43	17887m	13.765	ug/L	
14) Carbon disulfide	2.288	76	9771	0.251	ug/L #	92
15) Methyl Acetate	2.481	43	4335	1.167	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021022\
Data File : VV024588.D
Acq On : 10 Feb 2022 23:06
Operator : SY/MD
Sample : N1475-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M10

Manual IntegrationsAPPROVED

Quant Time: Feb 11 23:59:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 11 23:54:44 2022
Response via : Initial Calibration

Reviewed By :John Carlone 02/15/2022
Supervised By :Semsettin Yesilyurt 02/17/2022

