

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021022\
 Data File : VW024583.D
 Acq On : 10 Feb 2022 21:09
 Operator : SY/MD
 Sample : N1475-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4M03

Quant Time: Feb 11 23:58:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 11 23:54:44 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	120923	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	118066	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	59658	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	51087	5.040	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	100.800%	
7) Chloroethane-d5	1.561	69	45217	5.277	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	105.600%	
11) 1,1-Dichloroethene-d2	2.101	63	73094	3.297	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	66.000%	
20) 2-Butanone-d5	3.989	46	73329	43.579	ug/L	0.08
Spiked Amount	50.000	Range 40 - 130	Recovery	=	87.160%	
24) Chloroform-d	4.346	84	82721	4.637	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	92.800%	
26) 1,2-Dichloroethane-d4	5.034	65	40155	4.961	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	99.200%	
32) Benzene-d6	5.043	84	169471	5.059	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	101.200%	
36) 1,2-Dichloropropane-d6	6.069	67	51023	4.897	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	98.000%	
41) Toluene-d8	7.313	98	151113	4.837	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	96.800%	
43) trans-1,3-Dichloroprop...	7.625	79	17412	4.138	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	82.800%	
46) 2-Hexanone-d5	8.101	63	60281	40.665	ug/L	0.01
Spiked Amount	50.000	Range 45 - 130	Recovery	=	81.340%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	31869	5.137	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	102.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152	49610	5.159	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	103.200%	
Target Compounds					Qvalue	
13) Acetone	2.294	43	9895	7.452	ug/L	79
14) Carbon disulfide	2.288	76	3389	0.085	ug/L #	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021022\
Data File : VV024583.D
Acq On : 10 Feb 2022 21:09
Operator : SY/MD
Sample : N1475-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M03

Quant Time: Feb 11 23:58:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 11 23:54:44 2022
Response via : Initial Calibration




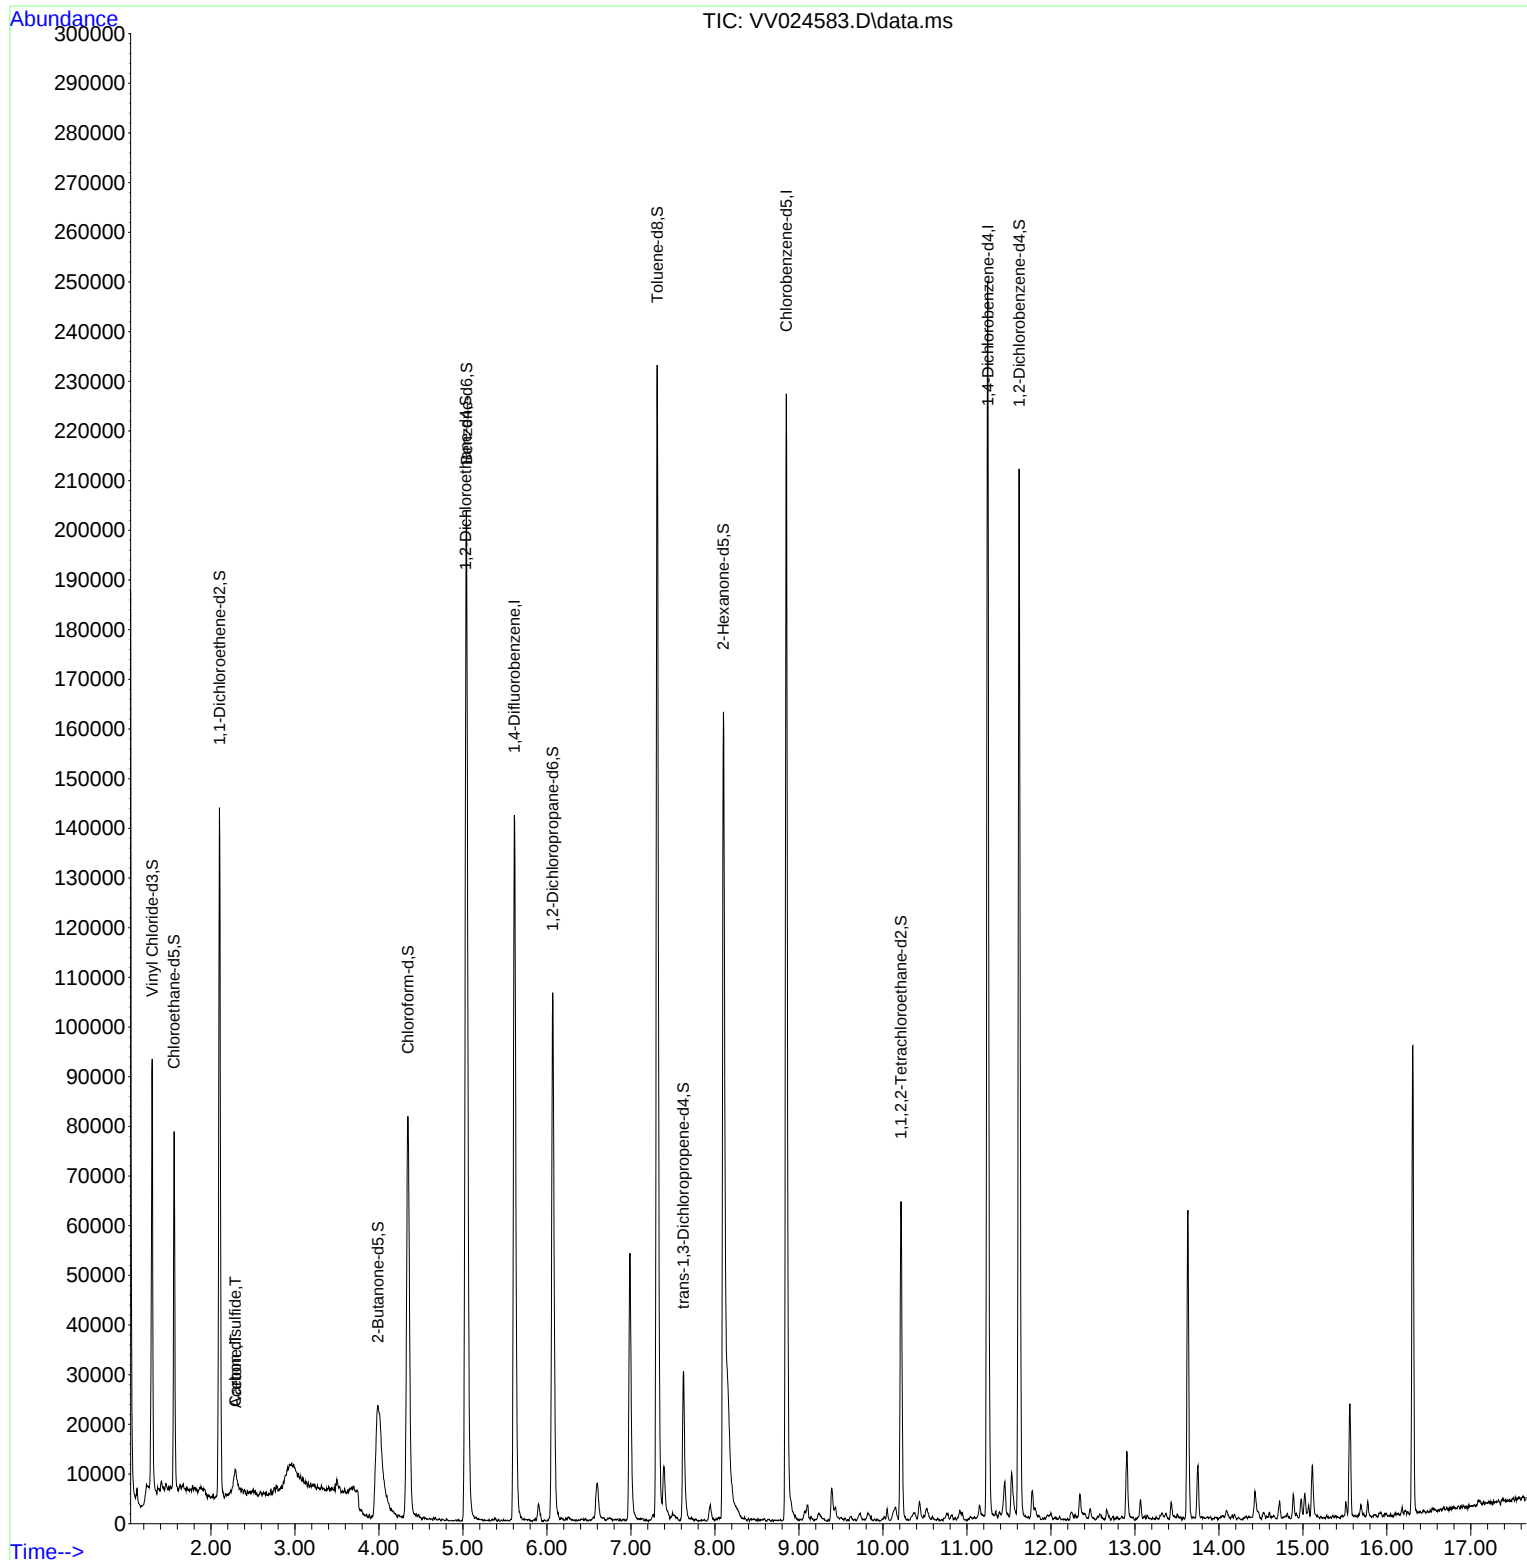


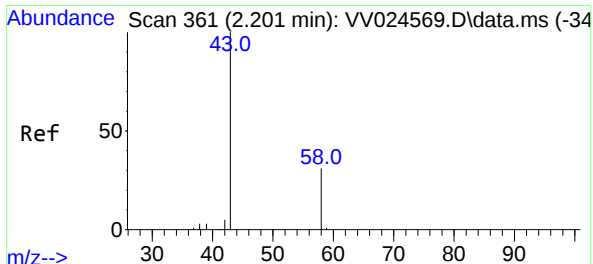

#13
Acetone
Concen: 7.452 ug/L
RT: 2.294 min Scan# 390
Delta R.T. 0.093 min
Lab File: VV024583.D
Acq: 10 Feb 2022 21:09

Instrument :
MSVOA_V
ClientSampleId :
F4M03

Tgt Ion: 43 Resp: 9895
Ion Ratio Lower Upper
43 100
58 10.8 0.0 41.4

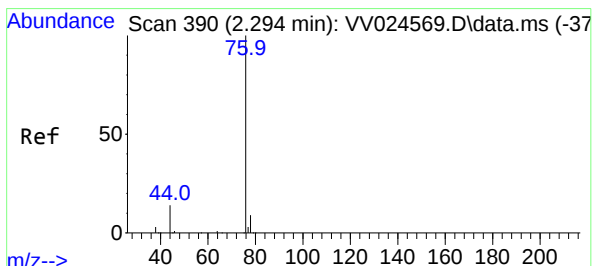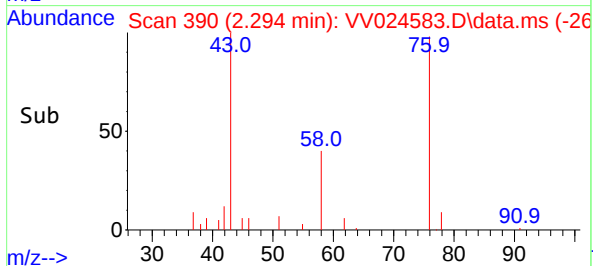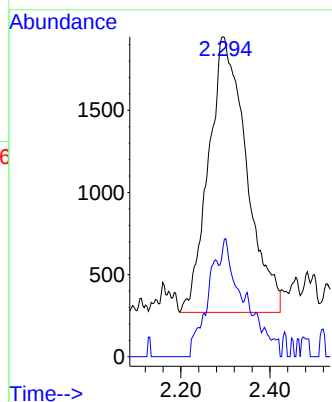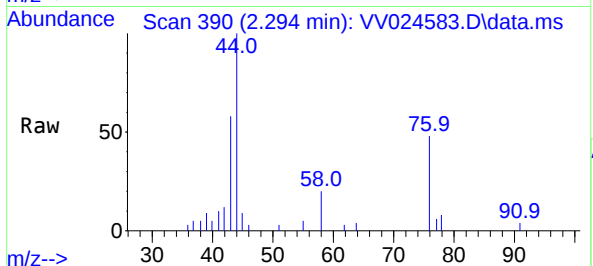

#14
Carbon disulfide
Concen: 0.085 ug/L
RT: 2.288 min Scan# 388
Delta R.T. -0.007 min
Lab File: VV024583.D
Acq: 10 Feb 2022 21:09

Tgt Ion: 76 Resp: 3389
Ion Ratio Lower Upper
76 100
78 14.5 7.5 11.3#

