

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021022\
 Data File : VW024585.D
 Acq On : 10 Feb 2022 21:56
 Operator : SY/MD
 Sample : N1475-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4M07

Quant Time: Feb 11 23:59:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 11 23:54:44 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	119722	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	118417	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	58516	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	51229	5.105	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	102.000%
7) Chloroethane-d5	1.561	69	44835	5.285	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	105.600%
11) 1,1-Dichloroethene-d2	2.102	63	73149	3.332	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.600%
20) 2-Butanone-d5	3.973	46	75796	45.497	ug/L	0.07
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.000%
24) Chloroform-d	4.346	84	83427	4.723	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.400%
26) 1,2-Dichloroethane-d4	5.037	65	39390	4.915	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.200%
32) Benzene-d6	5.047	84	164919	4.908	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.200%
36) 1,2-Dichloropropane-d6	6.069	67	50204	4.804	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.000%
41) Toluene-d8	7.314	98	150107	4.790	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.800%
43) trans-1,3-Dichloroprop...	7.625	79	17909	4.244	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.800%
46) 2-Hexanone-d5	8.098	63	62834	42.262	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.520%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	31660	5.088	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	101.800%
66) 1,2-Dichlorobenzene-d4	11.622	152	46057	4.883	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.600%
Target Compounds					Qvalue	
13) Acetone	2.278	43	15147	11.521	ug/L	80
14) Carbon disulfide	2.285	76	16087	0.408	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021022\
Data File : VV024585.D
Acq On : 10 Feb 2022 21:56
Operator : SY/MD
Sample : N1475-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M07

Quant Time: Feb 11 23:59:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 11 23:54:44 2022
Response via : Initial Calibration

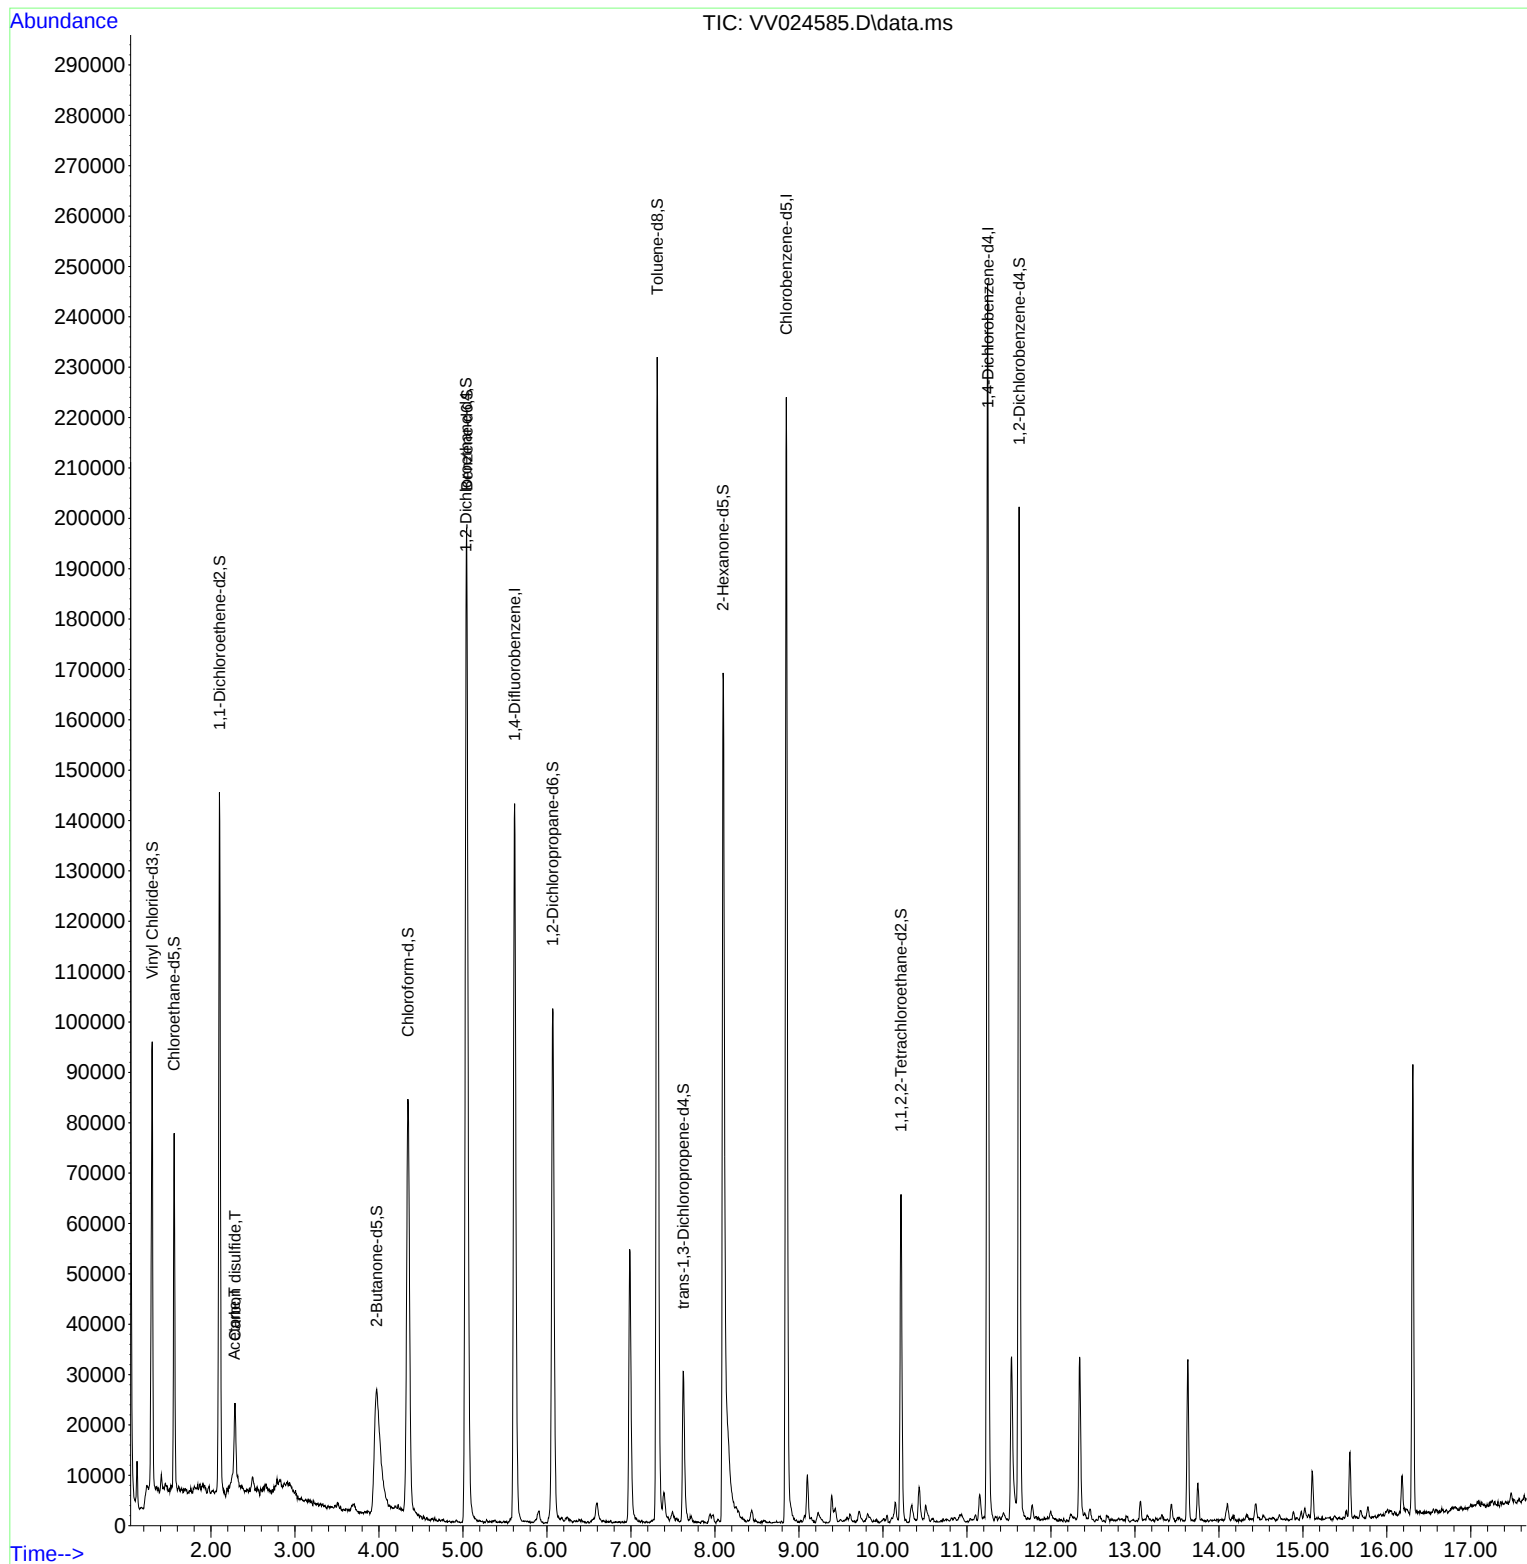

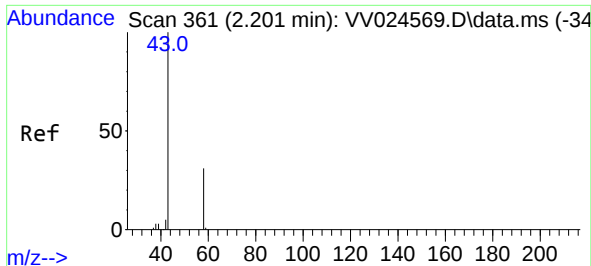

#13

Acetone

Concen: 11.521 ug/L

RT: 2.278 min Scan# 385

Delta R.T. 0.077 min

Lab File: VV024585.D

Acq: 10 Feb 2022 21:56

Instrument :

MSVOA_V

ClientSampleId :





F4M07

Tgt Ion: 43 Resp: 15147

Ion Ratio Lower Upper

43 100

58 11.5 0.0 41.4

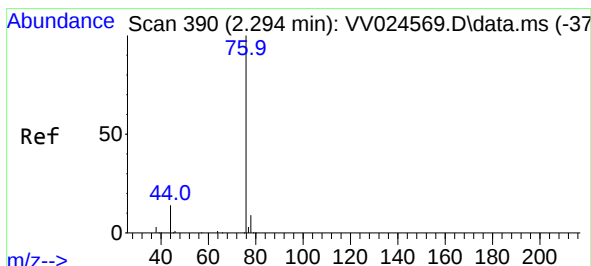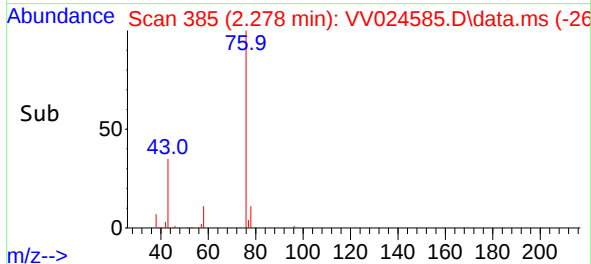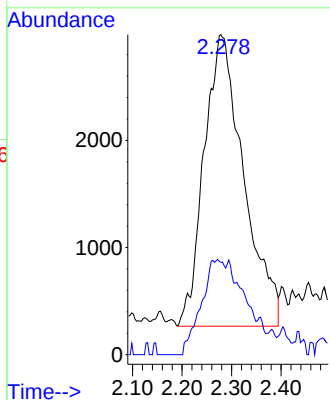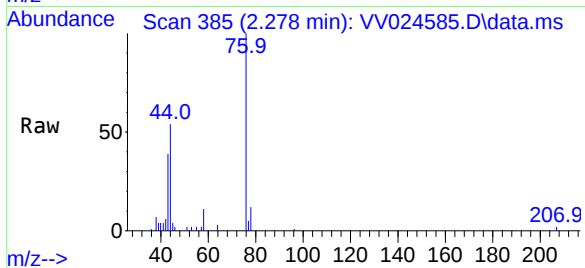

#14

Carbon disulfide

Concen: 0.408 ug/L

RT: 2.285 min Scan# 387

Delta R.T. -0.010 min

Lab File: VV024585.D

Acq: 10 Feb 2022 21:56

Tgt Ion: 76 Resp: 16087

Ion Ratio Lower Upper

76 100

78 10.0 7.5 11.3

