

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021022\
 Data File : VV024577.D
 Acq On : 10 Feb 2022 18:49
 Operator : SY/MD
 Sample : VIBLK251
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK251

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024577.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	99	rBV	75558	75722	15.08%	1.832%
2	1.571	157	165	175	rBV	69396	77969	15.53%	1.886%
3	2.111	322	333	350	rVB	139871	205820	40.99%	4.980%
4	2.510	449	457	465	rBV4	3285	5155	1.03%	0.125%
5	3.892	877	887	929	rBV	49126	158401	31.54%	3.832%
6	4.352	1011	1030	1058	rBV	88146	223500	44.51%	5.408%
7	5.050	1230	1247	1278	rBV2	201044	502157	100.00%	12.150%
8	5.619	1412	1424	1456	rBV	149078	301017	59.94%	7.283%
9	5.912	1506	1515	1530	rVB7	4707	10079	2.01%	0.244%
10	6.069	1552	1564	1590	rBV	115278	239984	47.79%	5.806%
11	6.989	1840	1850	1870	rBV	60852	113636	22.63%	2.749%
12	7.317	1941	1952	1971	rBV	251842	447589	89.13%	10.829%
13	7.400	1972	1978	1992	rVB5	3292	6667	1.33%	0.161%
14	7.625	2038	2048	2072	rBV	34069	62472	12.44%	1.511%
15	8.088	2182	2192	2229	rBV	232472	438292	87.28%	10.604%
16	8.850	2418	2429	2453	rBV	235898	390089	77.68%	9.438%
17	10.217	2842	2854	2871	rBV	67335	106400	21.19%	2.574%
18	11.246	3163	3174	3192	rBV	264633	409142	81.48%	9.899%
19	11.622	3280	3291	3313	rBV	228293	353180	70.33%	8.545%
20	14.181	4078	4087	4099	rVB5	3742	5858	1.17%	0.142%




Sum of corrected areas: 4133129

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021022\
Data File : VV024577.D
Acq On : 10 Feb 2022 18:49
Operator : SY/MD
Sample : VIBLK251
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK251

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

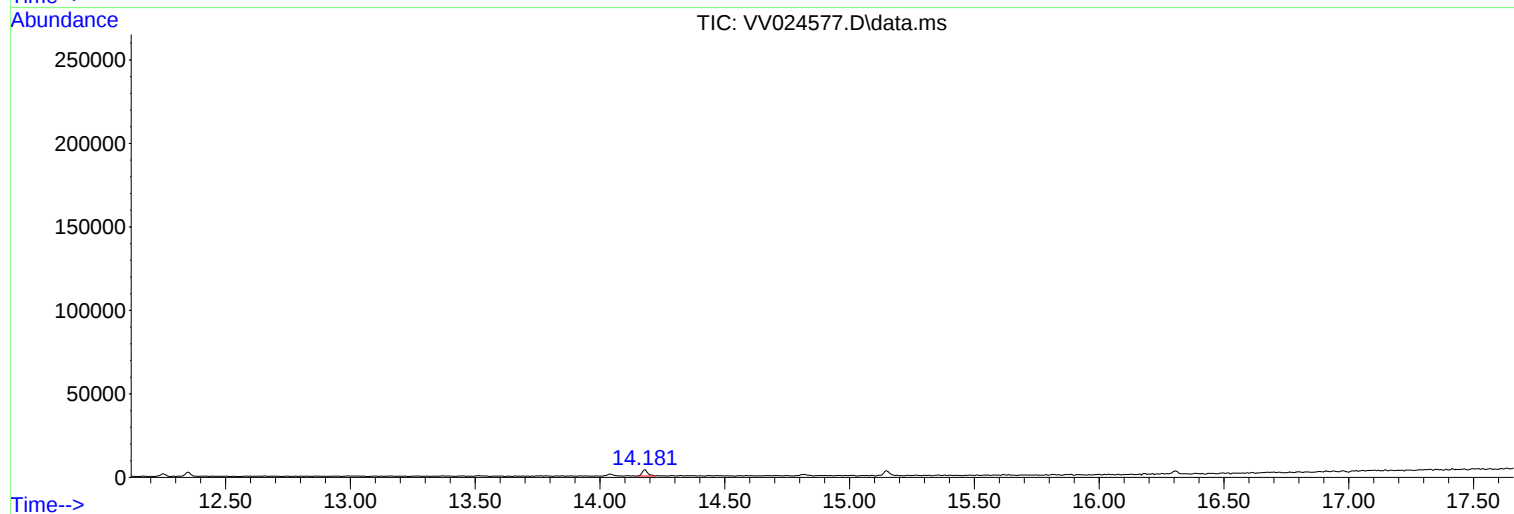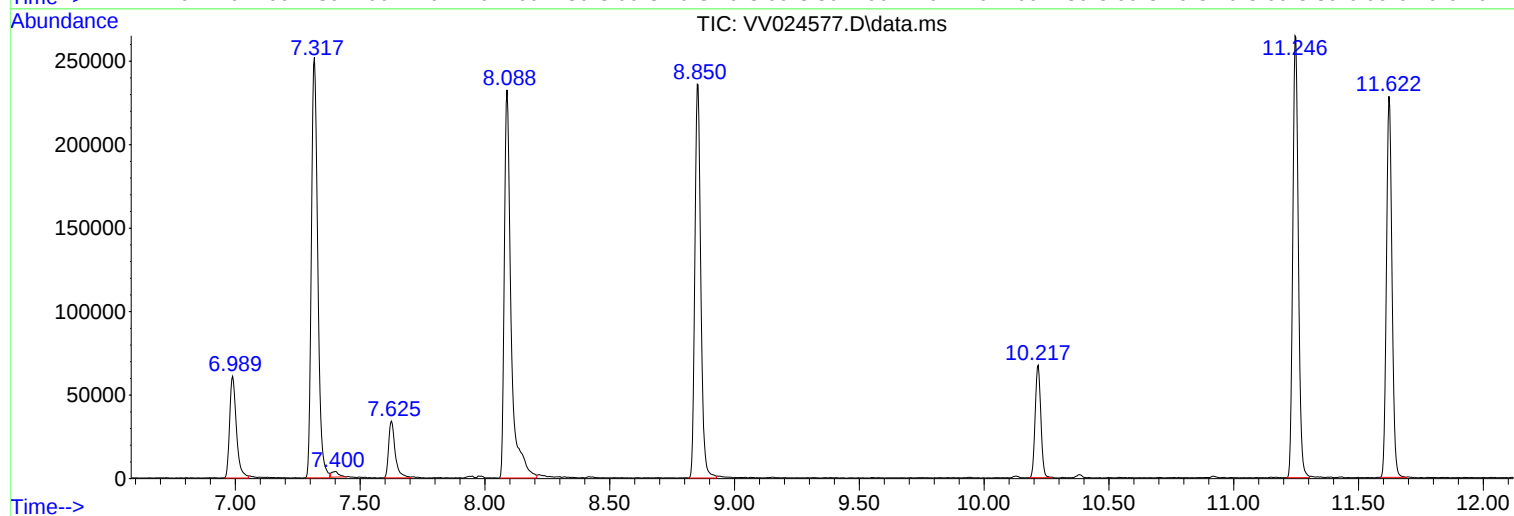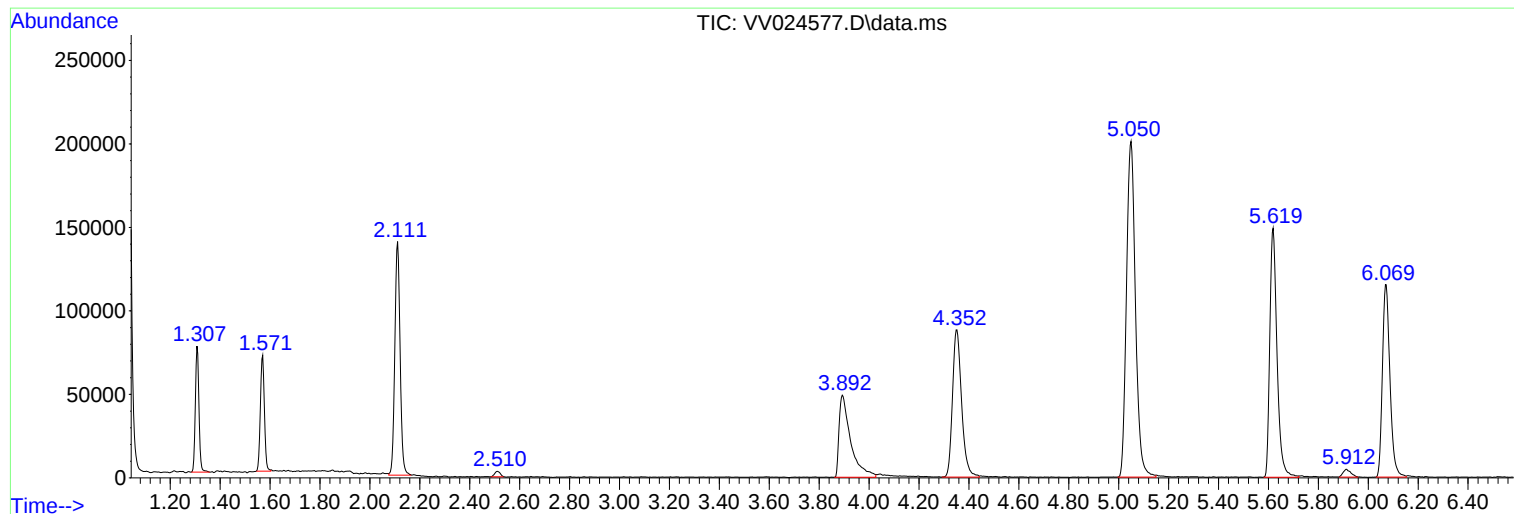

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021022\
Data File : VV024577.D
Acq On : 10 Feb 2022 18:49
Operator : SY/MD
Sample : VIBLK251
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK251

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021022\
Data File : VV024577.D
Acq On : 10 Feb 2022 18:49
Operator : SY/MD
Sample : VIBLK251
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK251

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc