

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021022\
 Data File : VV024589.D
 Acq On : 10 Feb 2022 23:29
 Operator : SY/MD
 Sample : N1475-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4M23

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024589.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	96	rVB	67793	70681	15.60%	1.869%
2	1.571	157	165	178	rBV	60665	68765	15.17%	1.818%
3	2.111	322	333	349	rVB	122624	179959	39.71%	4.757%
4	3.902	880	890	924	rBV2	31056	119874	26.45%	3.169%
5	4.352	1014	1030	1059	rVB	79564	197563	43.59%	5.223%
6	5.050	1230	1247	1279	rBV2	181453	453223	100.00%	11.981%
7	5.616	1409	1423	1448	rBV	138277	281727	62.16%	7.448%
8	5.912	1506	1515	1527	rVB5	2535	5101	1.13%	0.135%
9	6.069	1551	1564	1591	rBV	104673	216343	47.73%	5.719%
10	6.985	1839	1849	1882	rBV	53599	102733	22.67%	2.716%
11	7.317	1940	1952	1970	rBV	226720	397487	87.70%	10.508%
12	7.397	1972	1977	1992	rVB3	3734	7584	1.67%	0.200%
13	7.625	2038	2048	2075	rBV	31356	56843	12.54%	1.503%
14	8.088	2182	2192	2228	rBV	195663	403464	89.02%	10.666%
15	8.850	2418	2429	2460	rBV	222342	368247	81.25%	9.735%
16	10.214	2842	2853	2871	rBV	66868	106175	23.43%	2.807%
17	11.246	3163	3174	3194	rBV	254270	389599	85.96%	10.299%
18	11.535	3255	3264	3279	rBV2	7106	13698	3.02%	0.362%
19	11.622	3280	3291	3313	rVB	205811	323460	71.37%	8.551%
20	16.181	4700	4709	4720	rBV7	9442	14765	3.26%	0.390%
21	16.310	4741	4749	4754	rBV6	4162	5427	1.20%	0.143%




Sum of corrected areas: 3782718

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021022\
Data File : VV024589.D
Acq On : 10 Feb 2022 23:29
Operator : SY/MD
Sample : N1475-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

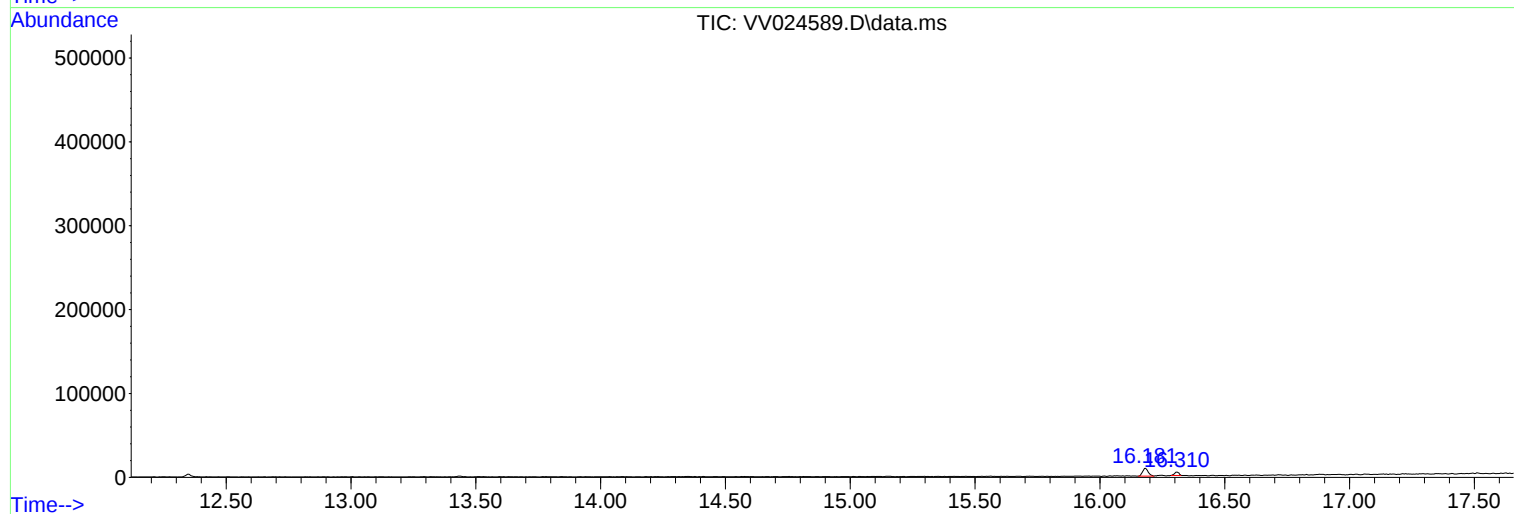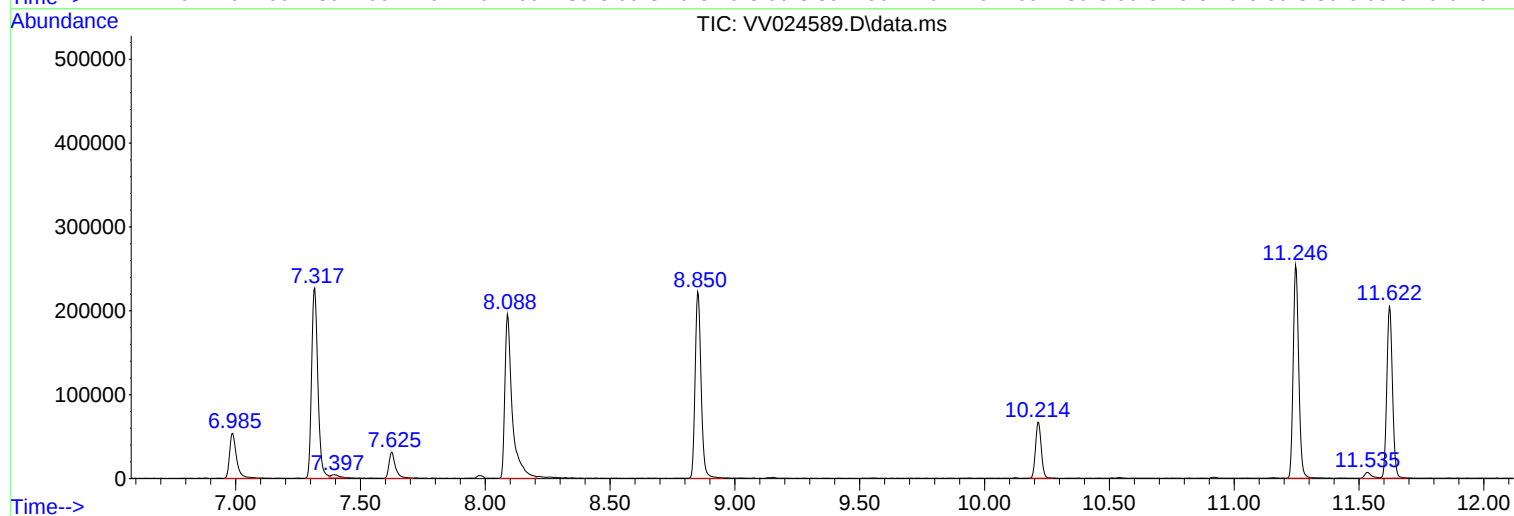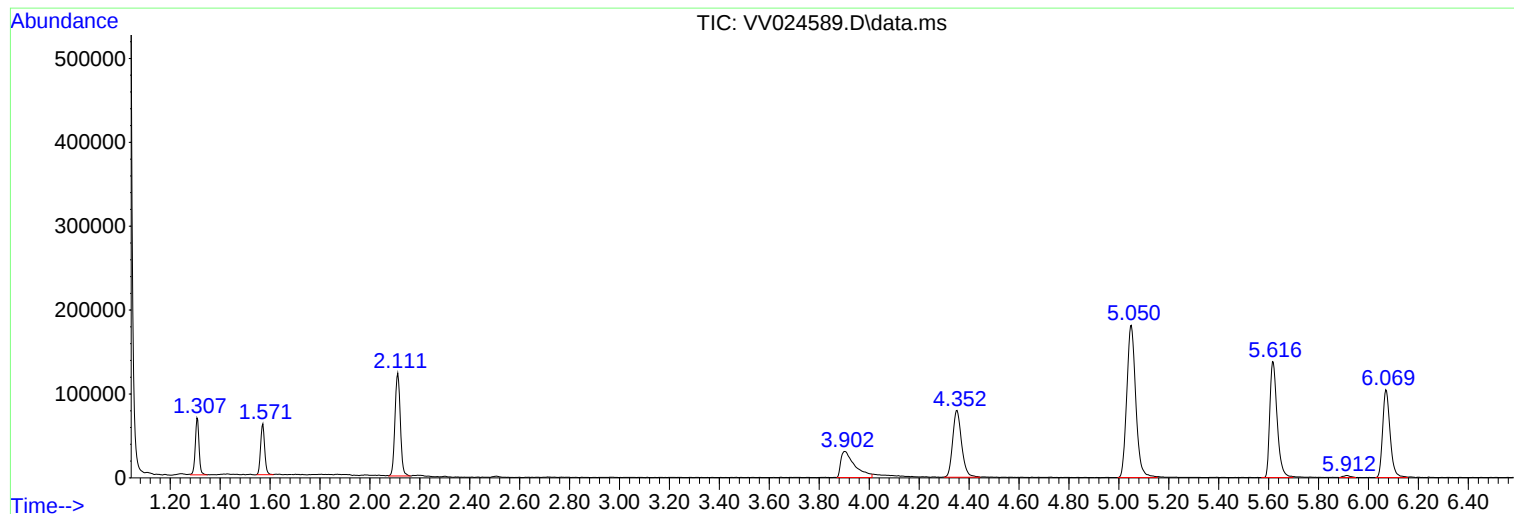

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021022\
Data File : VV024589.D
Acq On : 10 Feb 2022 23:29
Operator : SY/MD
Sample : N1475-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021022\
Data File : VV024589.D
Acq On : 10 Feb 2022 23:29
Operator : SY/MD
Sample : N1475-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc