




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV021025\
Data File : VV038672.D
Acq On : 10 Feb 2025 16:52
Operator : SY/MD
Sample : Q1335-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E29D4

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 02/14/2025
Supervised By :Mahesh Dadoda 02/18/2025

Quant Time: Feb 14 11:40:56 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020625WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 14 11:36:33 2025
Response via : Initial Calibration

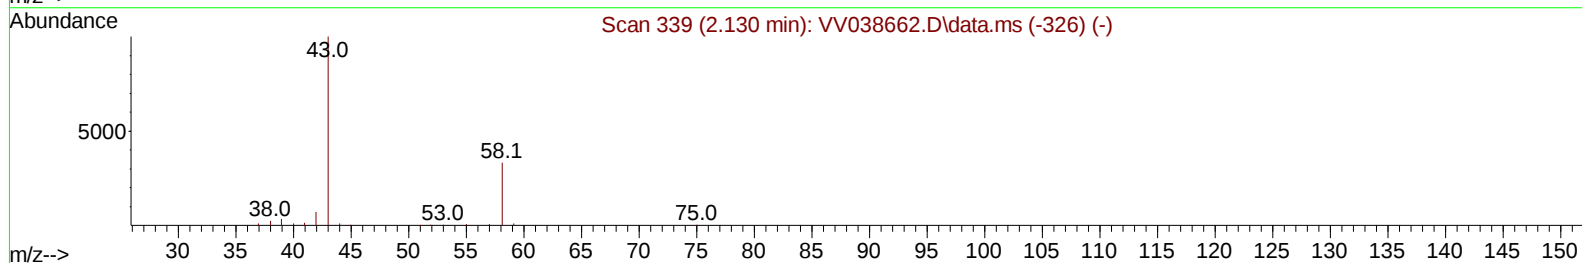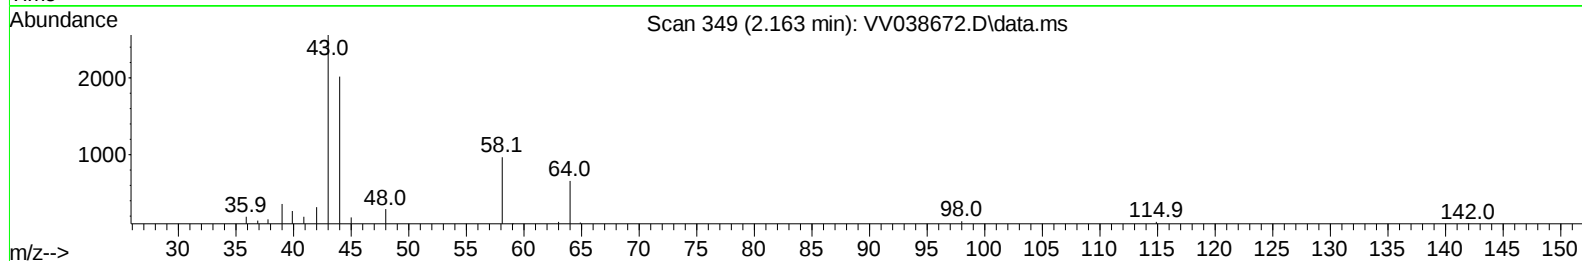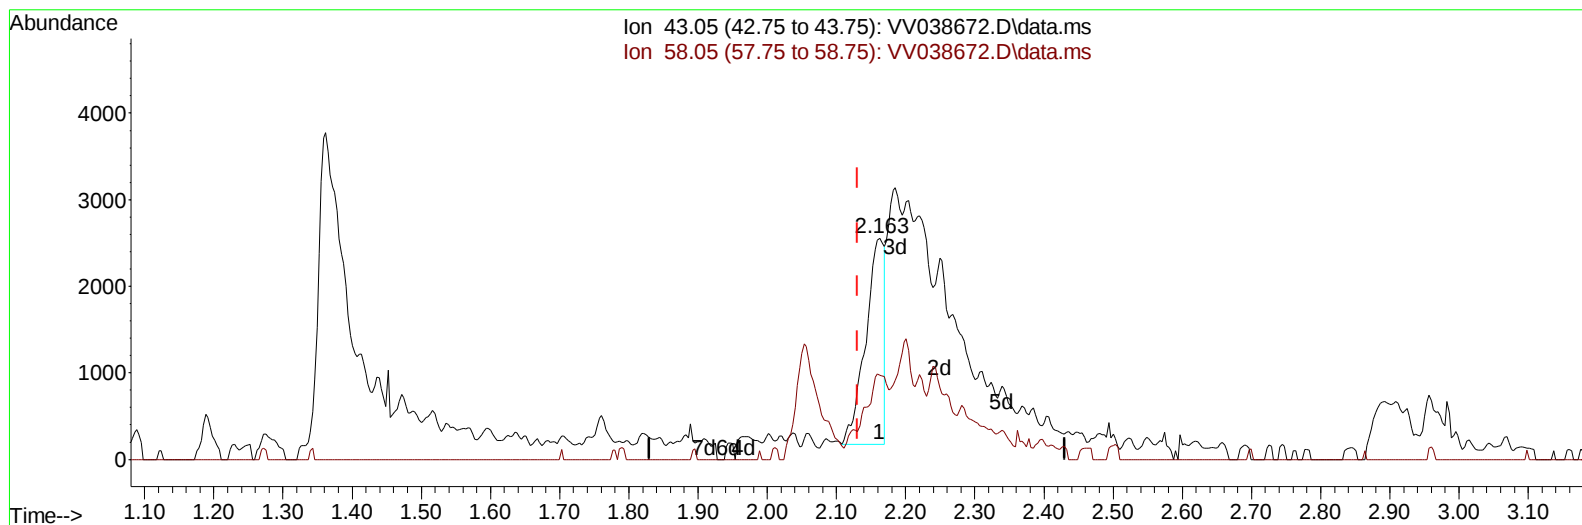

TIC: VV038672.D\data.ms

(13) Acetone (T)

2.163min (+ 0.032) 1.70 ug/L

response 4433

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	33.70	44.12
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV021025\
 Data File : VV038672.D
 Acq On : 10 Feb 2025 16:52
 Operator : SY/MD
 Sample : Q1335-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E29D4

Manual IntegrationsAPPROVED

Quant Time: Feb 14 11:40:56 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020625WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 14 11:36:33 2025
 Response via : Initial Calibration

Reviewed By :Romaben Patel 02/14/2025
 Supervised By :Mahesh Dadoda 02/18/2025

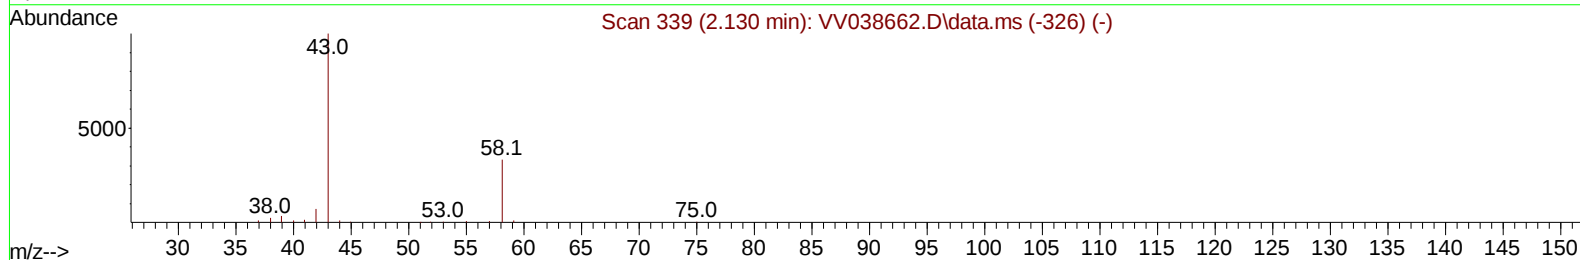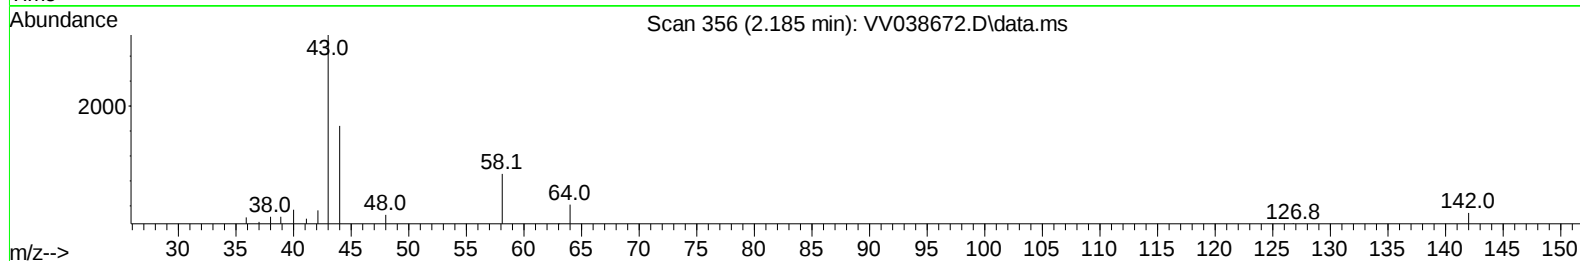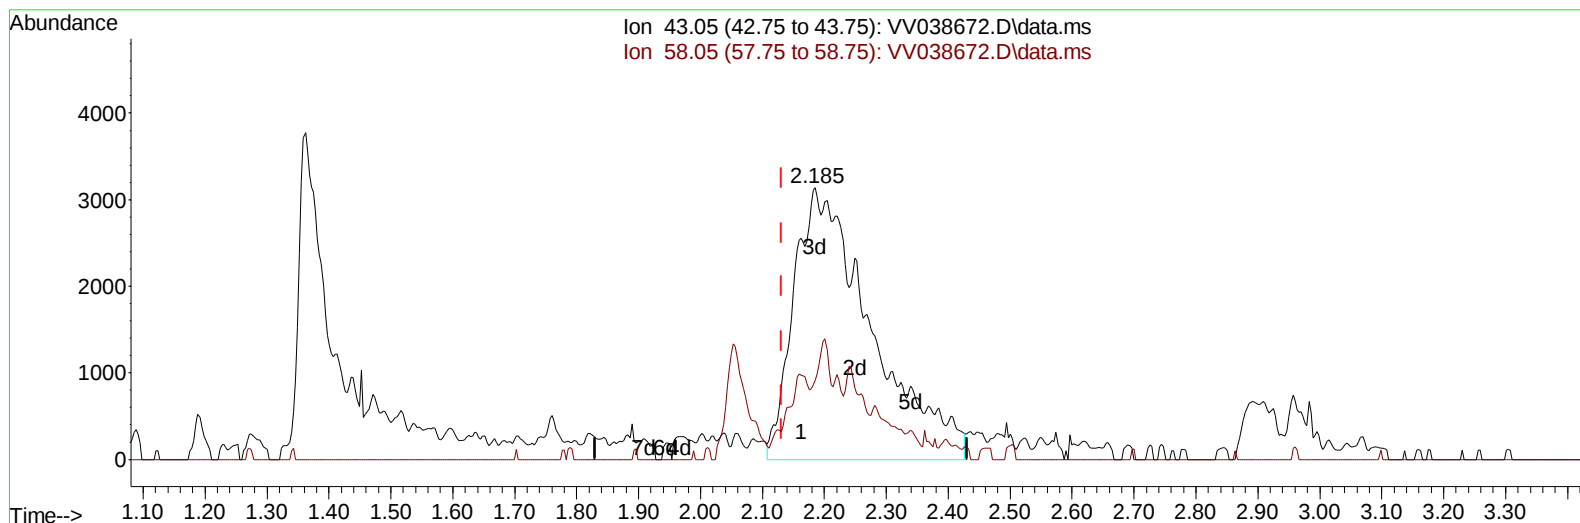

TIC: VV038672.D\data.ms

(13) Acetone (T)

2.185min (+ 0.055) 10.40 ug/L m

response 27158

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	33.70	7.20
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV021025\
Data File : VV038672.D
Acq On : 10 Feb 2025 16:52
Operator : SY/MD
Sample : Q1335-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E29D4

Manual IntegrationsAPPROVED

Quant Time: Feb 14 11:40:56 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020625WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 14 11:36:33 2025
Response via : Initial Calibration

Reviewed By :Romaben Patel 02/14/2025
Supervised By :Mahesh Dadoda 02/18/2025

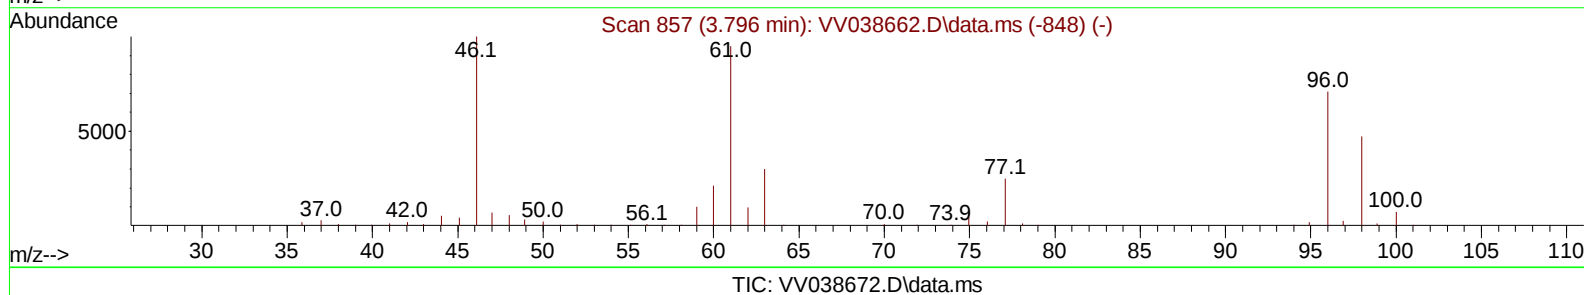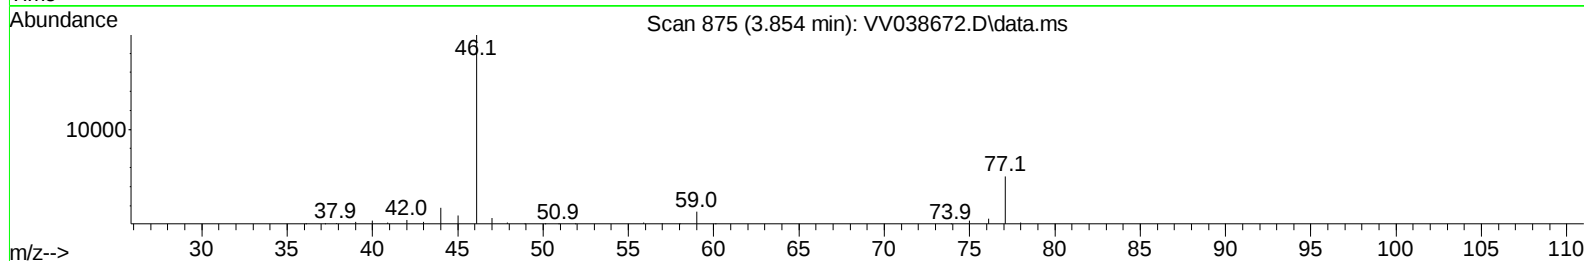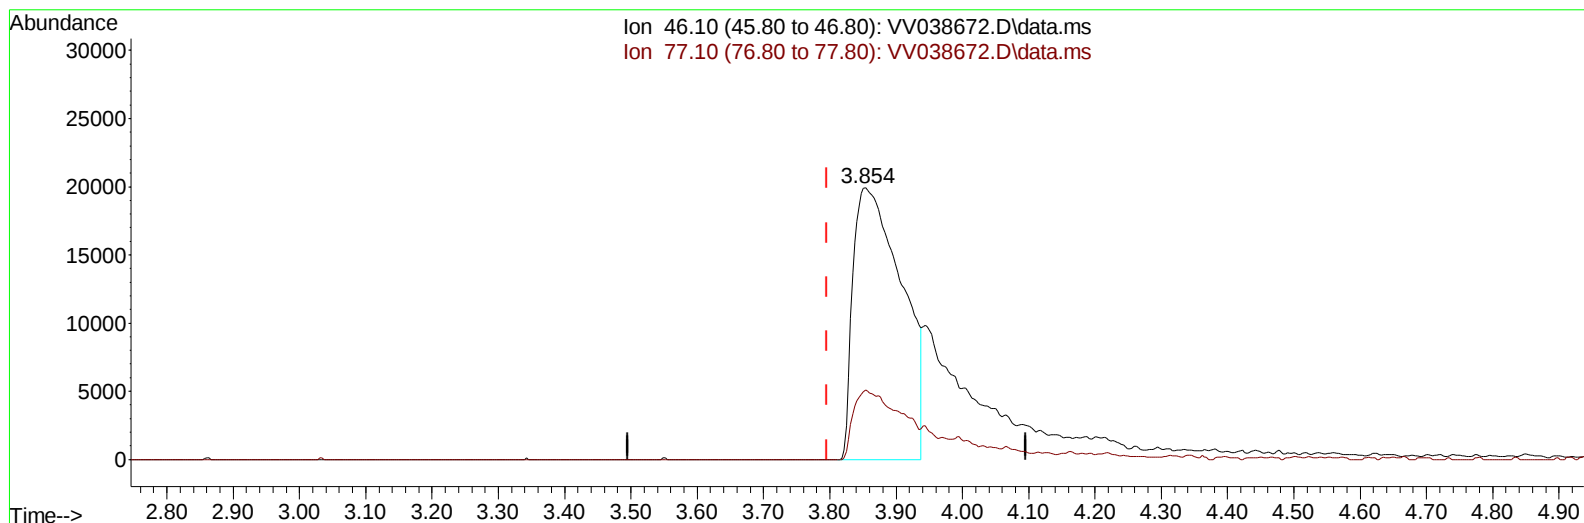

TIC: VV038672.D\data.ms

(20) 2-Butanone-d5 (S)

3.854min (+ 0.058) 28.60 ug/L

response 101718

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	23.70	24.56
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV021025\
Data File : VV038672.D
Acq On : 10 Feb 2025 16:52
Operator : SY/MD
Sample : Q1335-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E29D4

Manual IntegrationsAPPROVED

Quant Time: Feb 14 11:40:56 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020625WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 14 11:36:33 2025
Response via : Initial Calibration

Reviewed By :Romaben Patel 02/14/2025
Supervised By :Mahesh Dadoda 02/18/2025

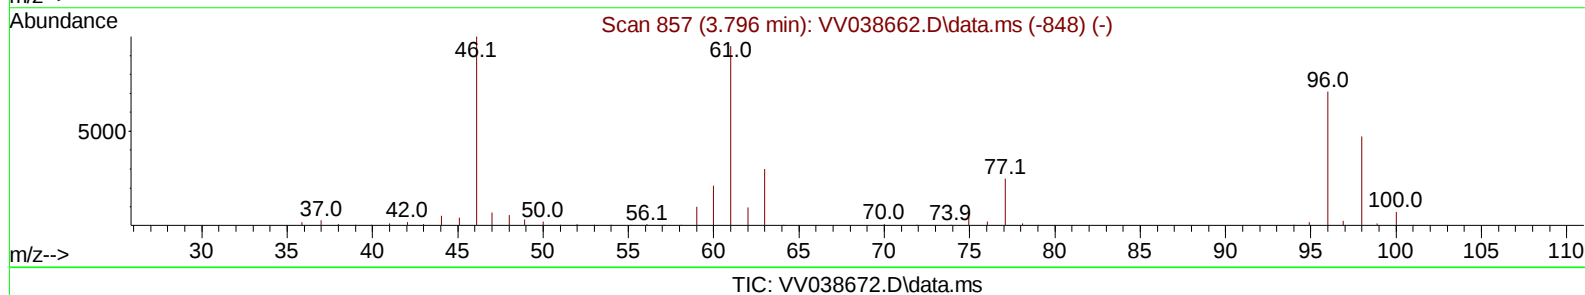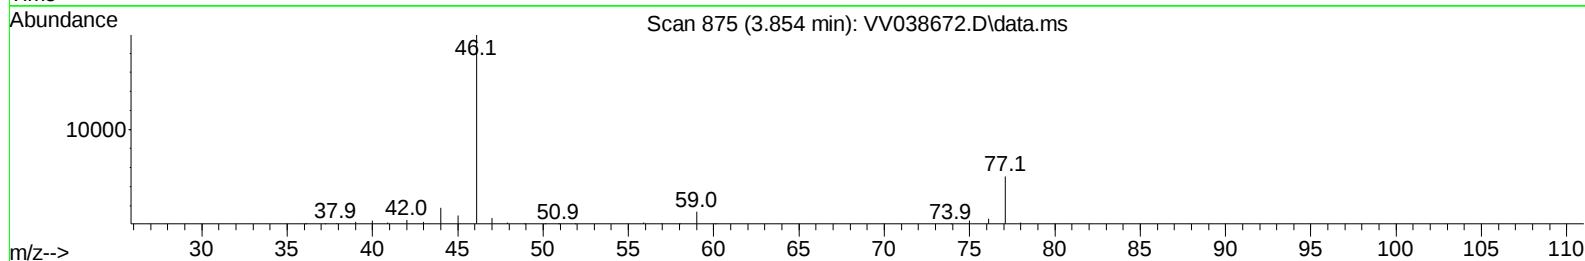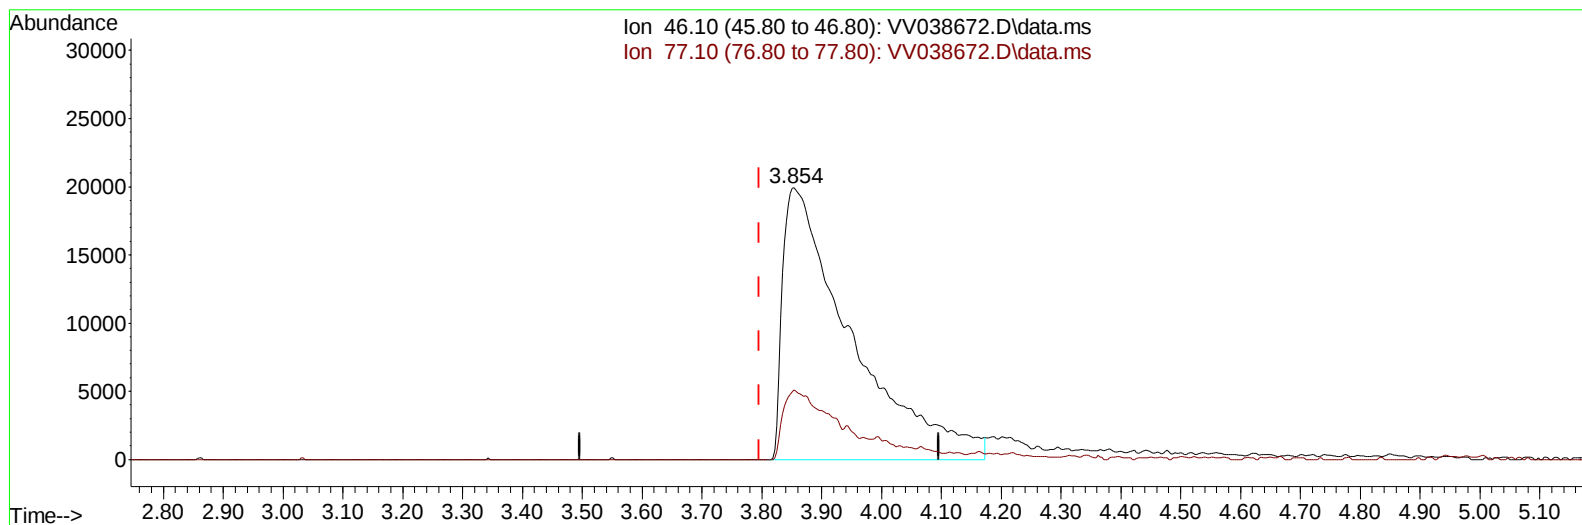

(20) 2-Butanone-d5 (S)

3.854min (+ 0.058) 44.54 ug/L m

response 158429

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	23.70	15.77#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV021025\
 Data File : VV038672.D
 Acq On : 10 Feb 2025 16:52
 Operator : SY/MD
 Sample : Q1335-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E29D4

Manual IntegrationsAPPROVED

Quant Time: Feb 14 11:40:56 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020625WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 14 11:36:33 2025
 Response via : Initial Calibration

Reviewed By :Romaben Patel 02/14/2025
 Supervised By :Mahesh Dadoda 02/18/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	198083	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	200395	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	89942	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	78808	3.85	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	77.00%	
7) Chloroethane-d5	1.529	69	64023	4.15	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	83.00%	
11) 1,1-Dichloroethene-d2	2.053	65	34514	4.03	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	80.60%	
20) 2-Butanone-d5	3.854	46	158429m	44.54	ug/L	0.06
Spiked Amount 50.000	Range 40	- 130	Recovery	=	89.08%	
24) Chloroform-d	4.243	84	141366	4.35	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	87.00%	
26) 1,2-Dichloroethane-d4	4.937	65	68837	4.82	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	96.40%	
32) Benzene-d6	4.953	84	270303	4.61	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	92.20%	
36) 1,2-Dichloropropane-d6	5.982	67	87679	5.05	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	101.00%	
41) Toluene-d8	7.236	98	219204	4.19	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	83.80%	
43) trans-1,3-Dichloroprop...	7.558	79	23833	3.74	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	74.80%	
46) 2-Hexanone-d5	8.027	63	128142	51.87	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	103.74%	
56) 1,1,2,2-Tetrachloroeth...	10.146	84	68554	4.64	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	92.80%	
66) 1,2-Dichlorobenzene-d4	11.554	152	81934	5.26	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	105.20%	
Target Compounds						
13) Acetone	2.185	43	27158m	10.40	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV021025\
Data File : VV038672.D
Acq On : 10 Feb 2025 16:52
Operator : SY/MD
Sample : Q1335-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E29D4

Manual IntegrationsAPPROVED

Quant Time: Feb 14 11:40:56 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020625WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 14 11:36:33 2025
Response via : Initial Calibration

Reviewed By :Romaben Patel 02/14/2025
Supervised By :Mahesh Dadoda 02/18/2025

