

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV021025\
 Data File : VV038672.D
 Acq On : 10 Feb 2025 16:52
 Operator : SY/MD
 Sample : Q1335-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E29D4

Manual Integrations
 APPROVED

Reviewed By :Romaben
 Patel

Quant Time: Feb 14 11:40:56 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020625WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 14 11:36:33 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	198083	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	200395	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	89942	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	78808	3.85	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	77.00%	
7) Chloroethane-d5	1.529	69	64023	4.15	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	83.00%	
11) 1,1-Dichloroethene-d2	2.053	65	34514	4.03	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	80.60%	
20) 2-Butanone-d5	3.854	46	158429m	44.54	ug/L	0.06
Spiked Amount	50.000	Range 40 - 130	Recovery	=	89.08%	
24) Chloroform-d	4.243	84	141366	4.35	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	87.00%	
26) 1,2-Dichloroethane-d4	4.937	65	68837	4.82	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	96.40%	
32) Benzene-d6	4.953	84	270303	4.61	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	92.20%	
36) 1,2-Dichloropropane-d6	5.982	67	87679	5.05	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	101.00%	
41) Toluene-d8	7.236	98	219204	4.19	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	83.80%	
43) trans-1,3-Dichloroprop...	7.558	79	23833	3.74	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	74.80%	
46) 2-Hexanone-d5	8.027	63	128142	51.87	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	103.74%	
56) 1,1,2,2-Tetrachloroeth...	10.146	84	68554	4.64	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	92.80%	
66) 1,2-Dichlorobenzene-d4	11.554	152	81934	5.26	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	105.20%	
Target Compounds						
13) Acetone	2.185	43	27158m	10.40	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV021025\
Data File : VV038672.D
Acq On : 10 Feb 2025 16:52
Operator : SY/MD
Sample : Q1335-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
E29D4

Quant Time: Feb 14 11:40:56 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020625WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 14 11:36:33 2025
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Romaben
Patel

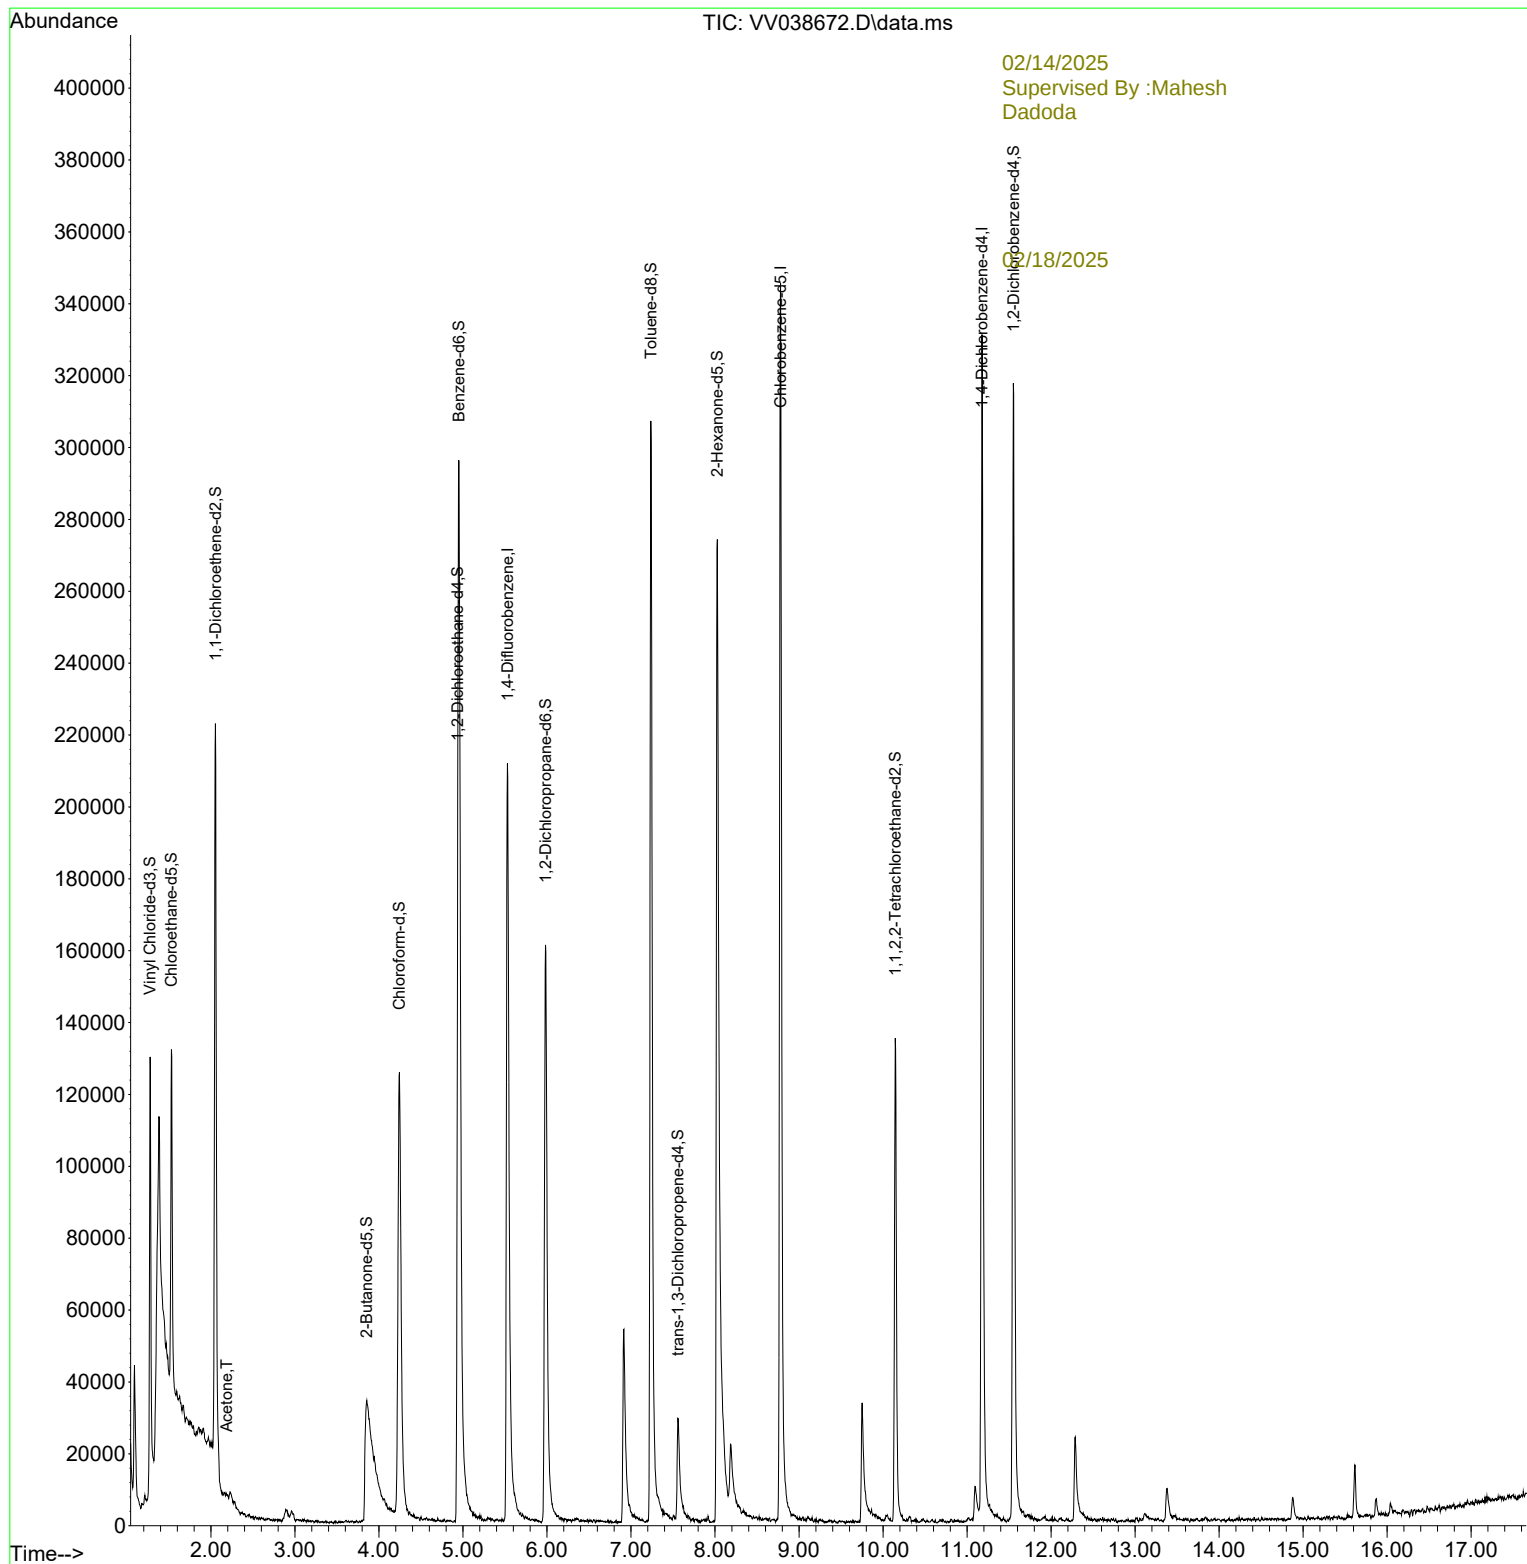

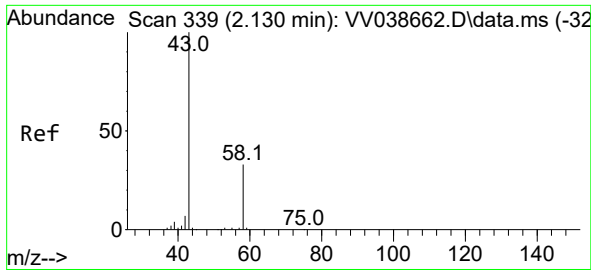

#13
Acetone
Concen: 10.40 ug/L m
RT: 2.185 min Scan# 3
Delta R.T. 0.055 min
Lab File: VV038672.D
Acq: 10 Feb 2025 16:52



Instrument :
MSVOA_V
ClientSampleId :
E29D4

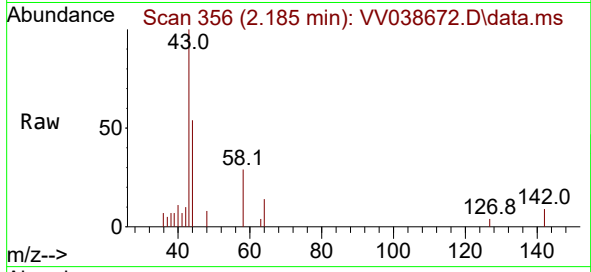

Tgt Ion: 43 Resp: 27158
Ion Ratio Lower Upper
43 100
58 7.2 0.0 67.4

Manual Integrations
APPROVED

Reviewed By :Romaben
Patel

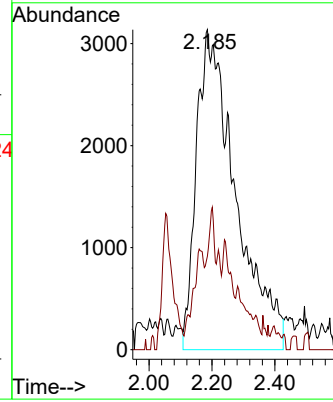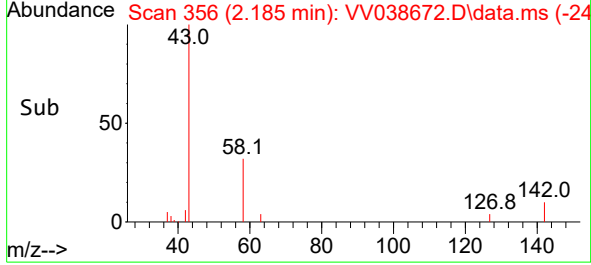

02/14/2025
Supervised By :Mahesh
Dadoda

02/18/2025