

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV021025\
 Data File : VV038664.D
 Acq On : 10 Feb 2025 13:36
 Operator : SY/MD
 Sample : Q1335-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E29C3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020625WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV038664.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.188	39	46	66	rBV	35905	86309	9.27%	1.081%
2	1.282	67	75	84	rBV	137615	147051	15.79%	1.841%
3	1.336	84	92	104	rBV	43340	107007	11.49%	1.340%
4	1.532	146	153	166	rBV	114884	140148	15.04%	1.755%
5	2.057	306	316	331	rVB	241162	356213	38.24%	4.461%
6	3.799	847	858	894	rBV	81545	274139	29.43%	3.433%
7	4.240	980	995	1021	rBV	149546	395230	42.43%	4.949%
8	4.947	1201	1215	1245	rBV2	350188	904426	97.09%	11.325%
9	5.526	1383	1395	1428	rBV	335068	731277	78.50%	9.157%
10	5.979	1522	1536	1563	rBV	190252	426624	45.80%	5.342%
11	6.912	1816	1826	1856	rBV	75448	173357	18.61%	2.171%
12	7.236	1916	1927	1955	rBV	388938	733145	78.70%	9.180%
13	7.555	2018	2026	2050	rBV2	40798	90974	9.77%	1.139%
14	8.021	2162	2171	2214	rBV	315383	736635	79.08%	9.224%
15	8.776	2395	2406	2437	rBV	529249	931537	100.00%	11.665%
16	10.146	2818	2832	2853	rBV	140874	235024	25.23%	2.943%
17	11.178	3143	3153	3180	rBV	497055	819048	87.92%	10.256%
18	11.551	3258	3269	3296	rBV	358940	614214	65.94%	7.691%
19	14.873	4292	4302	4315	rBV3	10285	18489	1.98%	0.232%
20	15.609	4522	4531	4545	rBV	30326	50283	5.40%	0.630%
21	15.866	4603	4611	4619	rBV2	9944	14797	1.59%	0.185%




Sum of corrected areas: 7985927

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV021025\
Data File : VV038664.D
Acq On : 10 Feb 2025 13:36
Operator : SY/MD
Sample : Q1335-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E29C3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020625WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

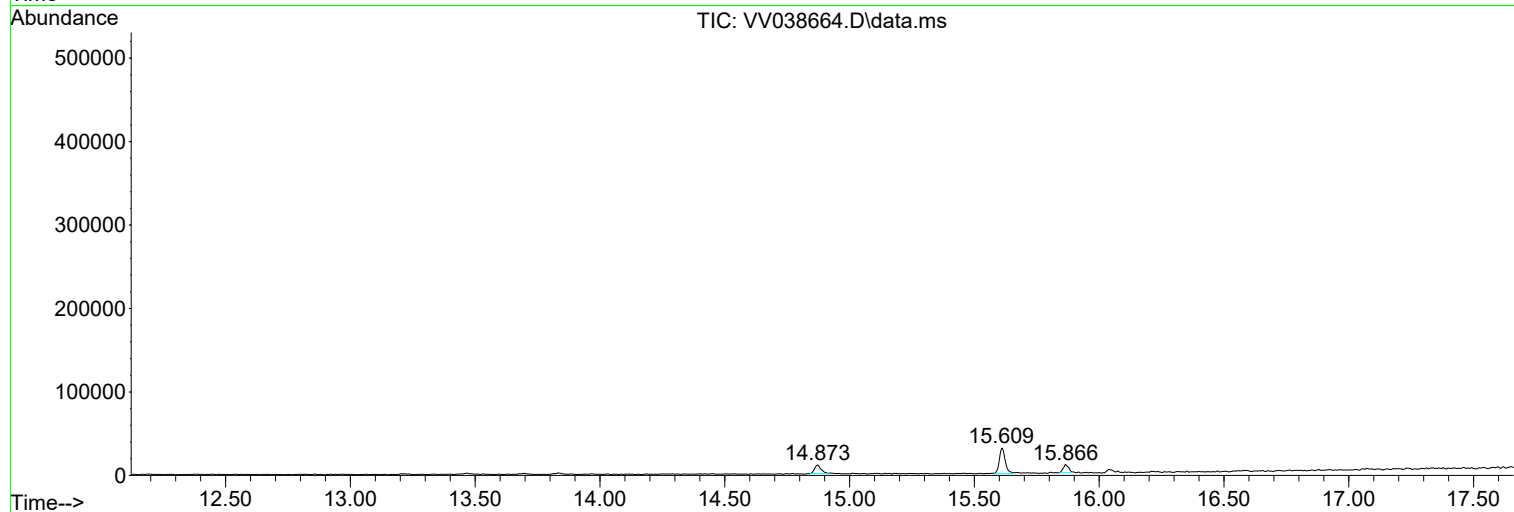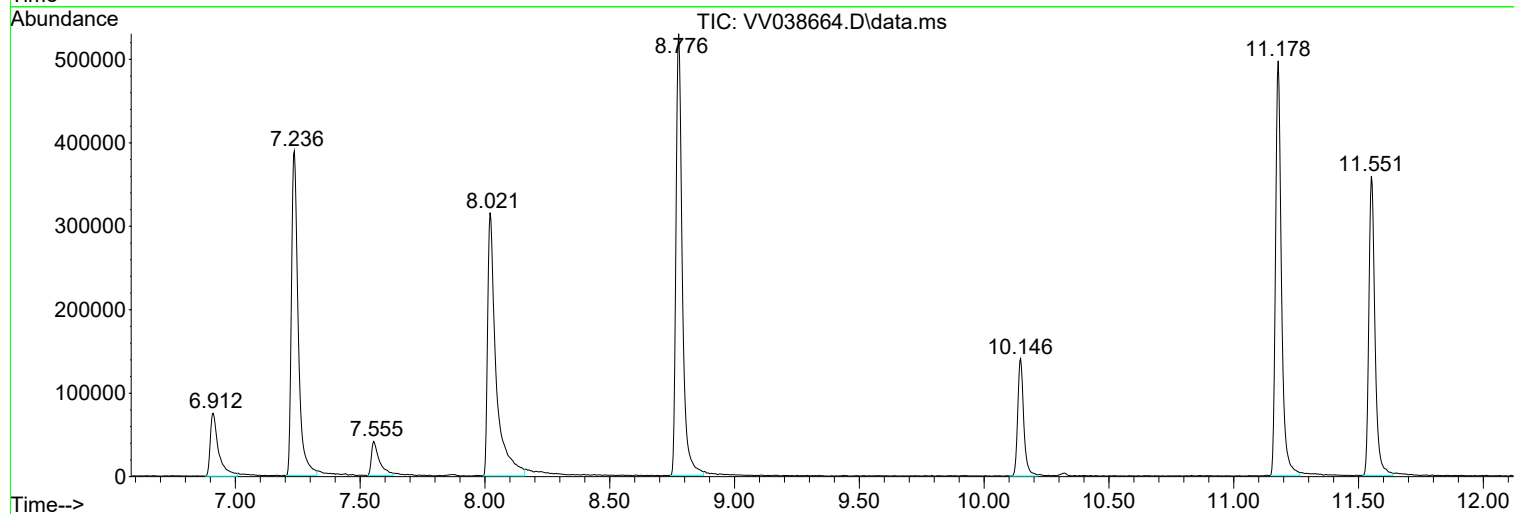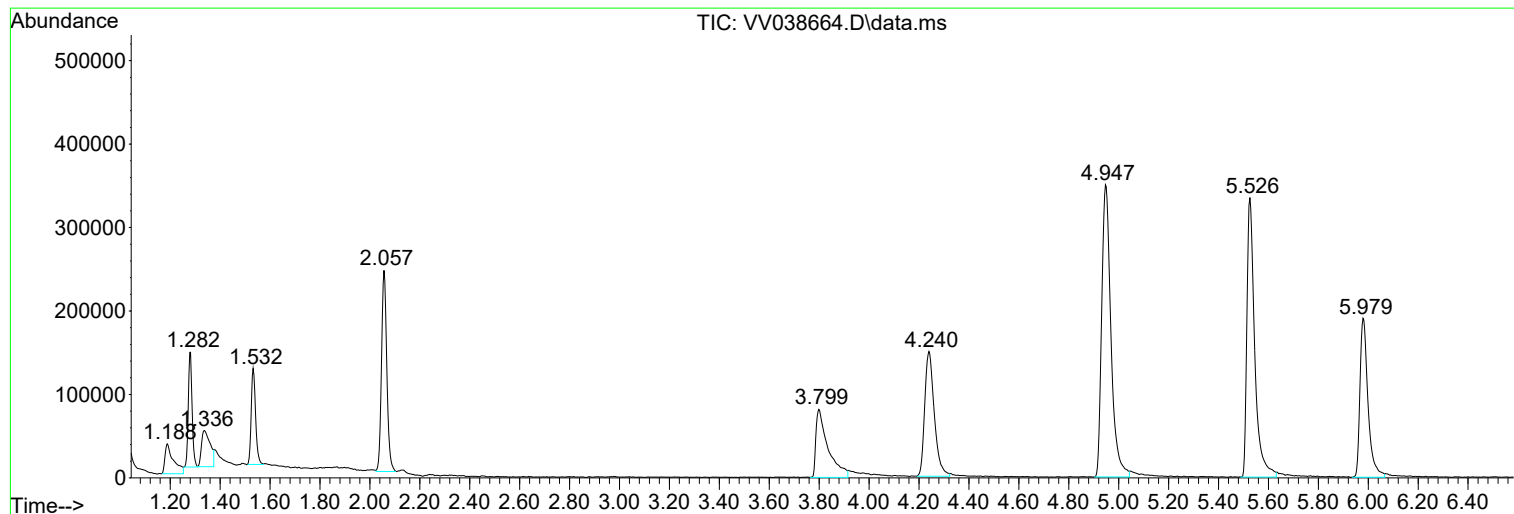

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV021025\
Data File : VV038664.D
Acq On : 10 Feb 2025 13:36
Operator : SY/MD
Sample : Q1335-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E29C3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020625WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV021025\
Data File : VV038664.D
Acq On : 10 Feb 2025 13:36
Operator : SY/MD
Sample : Q1335-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E29C3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020625WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc