

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV021025\
 Data File : VV038667.D
 Acq On : 10 Feb 2025 14:48
 Operator : SY/MD
 Sample : Q1335-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E29C6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020625WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV038667.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.185	38	45	65	rBV	45826	95849	11.70%	1.316%
2	1.278	67	74	78	rBV	129900	135622	16.55%	1.862%
3	1.317	78	86	103	rVV	257362	502039	61.26%	6.892%
4	1.532	147	153	169	rVB	107592	138841	16.94%	1.906%
5	2.056	307	316	335	rVB	225537	375943	45.88%	5.161%
6	3.799	849	858	884	rBV	82218	259100	31.62%	3.557%
7	4.240	978	995	1025	rBV2	131344	351306	42.87%	4.822%
8	4.950	1201	1216	1255	rBV2	310809	819467	100.00%	11.249%
9	5.529	1384	1396	1436	rBV	229029	515779	62.94%	7.080%
10	5.982	1524	1537	1565	rBV	173350	386400	47.15%	5.304%
11	6.915	1817	1827	1850	rBV	59536	131632	16.06%	1.807%
12	7.236	1917	1927	1963	rBV	335000	642558	78.41%	8.821%
13	7.558	2020	2027	2051	rBV2	29992	67915	8.29%	0.932%
14	8.021	2163	2171	2214	rBV	345004	778592	95.01%	10.688%
15	8.776	2396	2406	2439	rBV	376442	669818	81.74%	9.195%
16	10.146	2820	2832	2851	rBV2	139626	231749	28.28%	3.181%
17	11.178	3141	3153	3180	rBV	344558	585279	71.42%	8.034%
18	11.551	3258	3269	3290	rBV	326054	548661	66.95%	7.532%
19	14.876	4294	4303	4313	rBV2	7323	12659	1.54%	0.174%
20	15.615	4525	4533	4546	rBV3	16998	26360	3.22%	0.362%
21	15.869	4603	4612	4620	rBV6	5740	9192	1.12%	0.126%




Sum of corrected areas: 7284761

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV021025\
Data File : VV038667.D
Acq On : 10 Feb 2025 14:48
Operator : SY/MD
Sample : Q1335-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E29C6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020625WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

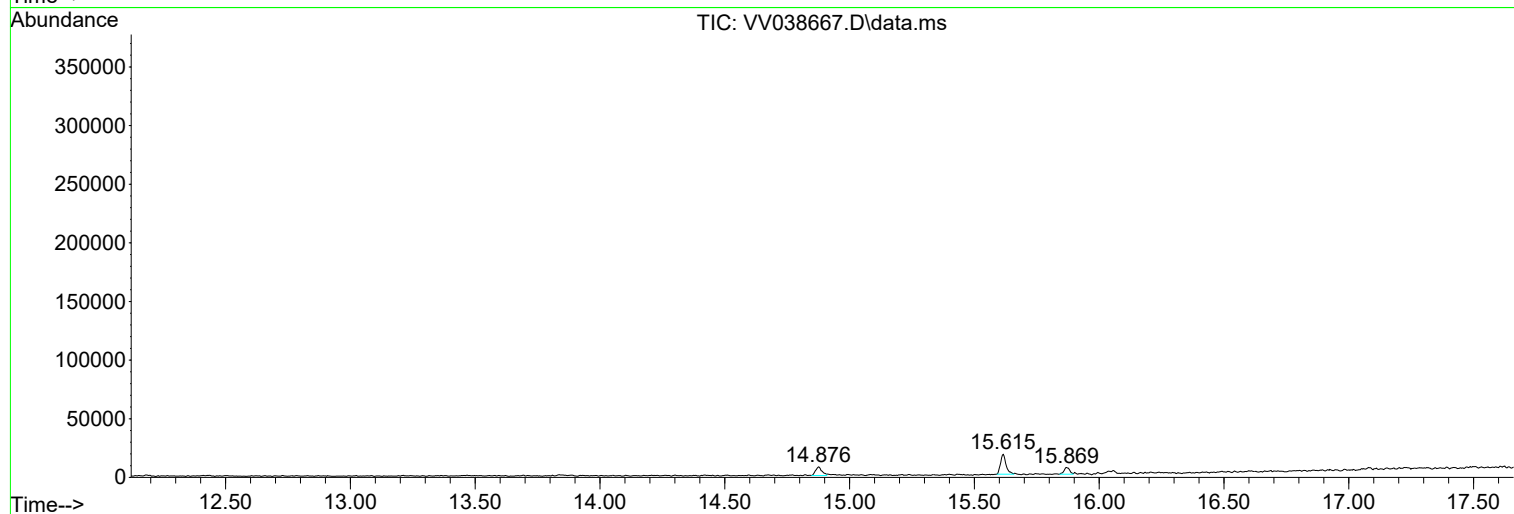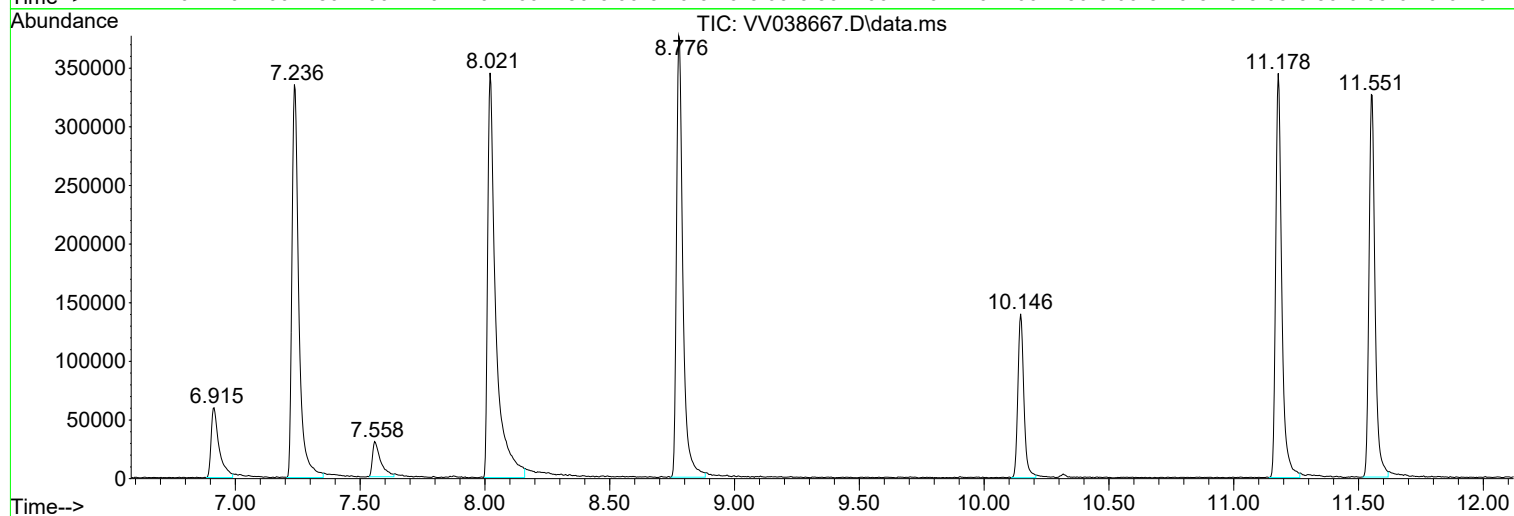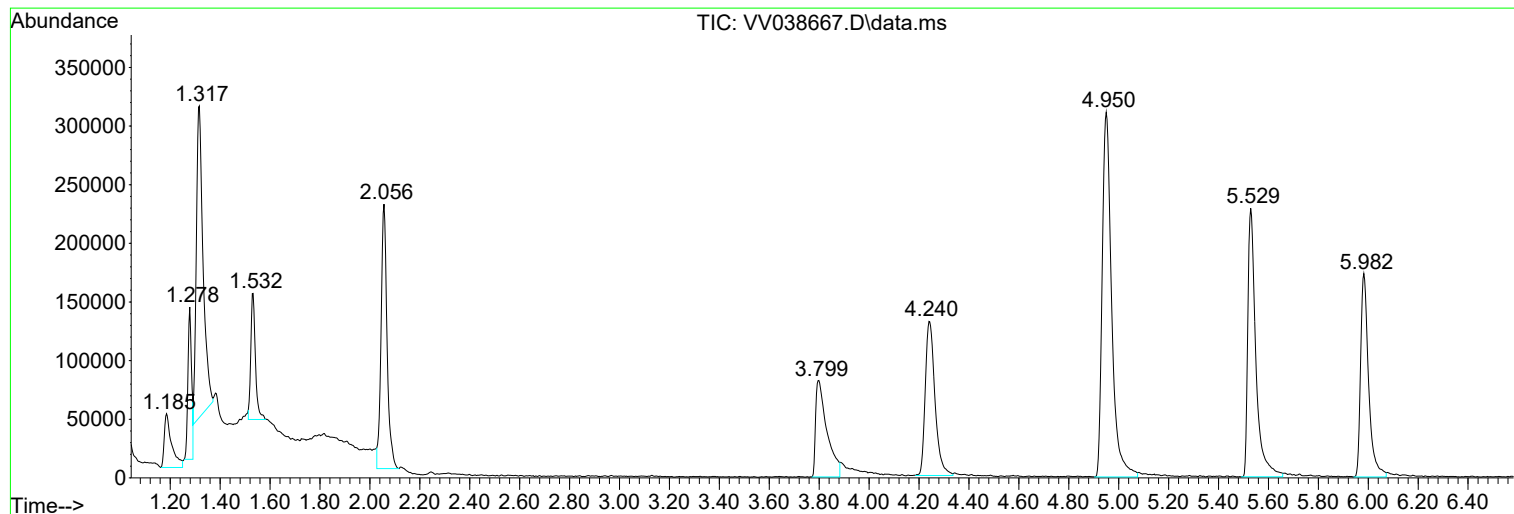

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV021025\
Data File : VV038667.D
Acq On : 10 Feb 2025 14:48
Operator : SY/MD
Sample : Q1335-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E29C6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020625WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV021025\
Data File : VV038667.D
Acq On : 10 Feb 2025 14:48
Operator : SY/MD
Sample : Q1335-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E29C6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020625WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc