

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV021025\
 Data File : VV038670.D
 Acq On : 10 Feb 2025 16:03
 Operator : SY/MD
 Sample : Q1335-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E29D0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020625WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV038670.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.185	38	45	65	rBV	50088	108542	13.98%	1.598%
2	1.278	67	74	81	rVV	117863	124649	16.05%	1.835%
3	1.323	81	88	102	rVV	115712	251944	32.44%	3.710%
4	1.384	104	107	117	rVB	38536	46852	6.03%	0.690%
5	1.532	146	153	166	rBV	99821	119197	15.35%	1.755%
6	2.056	306	316	332	rVB	208738	319981	41.20%	4.711%
7	3.799	849	858	887	rBV2	80311	256704	33.06%	3.780%
8	4.243	979	996	1025	rBV	128334	341252	43.94%	5.024%
9	4.950	1202	1216	1254	rBV3	296844	776559	100.00%	11.434%
10	5.529	1385	1396	1430	rBV	227482	514365	66.24%	7.573%
11	5.982	1524	1537	1566	rBV2	166932	372068	47.91%	5.478%
12	6.915	1817	1827	1845	rBV2	60059	127821	16.46%	1.882%
13	7.236	1915	1927	1967	rBV	319177	614353	79.11%	9.045%
14	7.558	2015	2027	2046	rBV	32863	73530	9.47%	1.083%
15	8.021	2162	2171	2209	rBV	327665	737261	94.94%	10.855%
16	8.780	2397	2407	2444	rBV	371277	664767	85.60%	9.788%
17	10.146	2821	2832	2854	rBV	133632	223134	28.73%	3.285%
18	11.178	3141	3153	3178	rBV	339961	571465	73.59%	8.414%
19	11.555	3254	3270	3297	rBV	301073	518063	66.71%	7.628%
20	14.879	4296	4304	4310	rBV4	6098	9369	1.21%	0.138%
21	15.615	4525	4533	4544	rBV2	11775	19978	2.57%	0.294%




Sum of corrected areas: 6791854

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV021025\
Data File : VV038670.D
Acq On : 10 Feb 2025 16:03
Operator : SY/MD
Sample : Q1335-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E29D0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020625WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

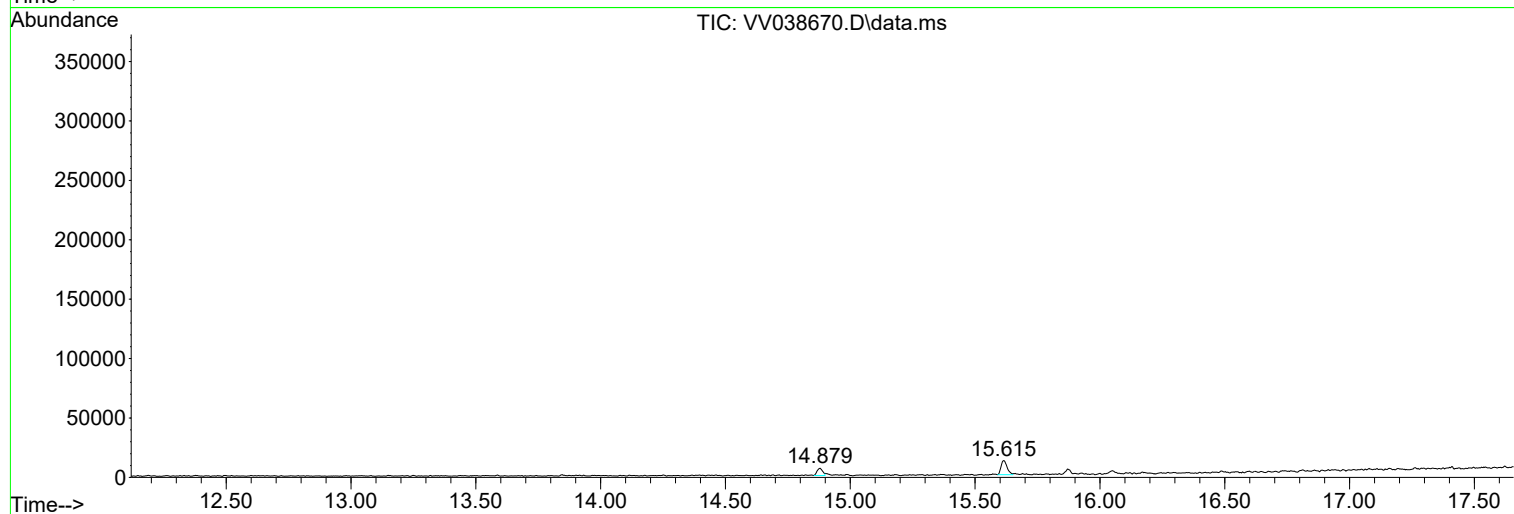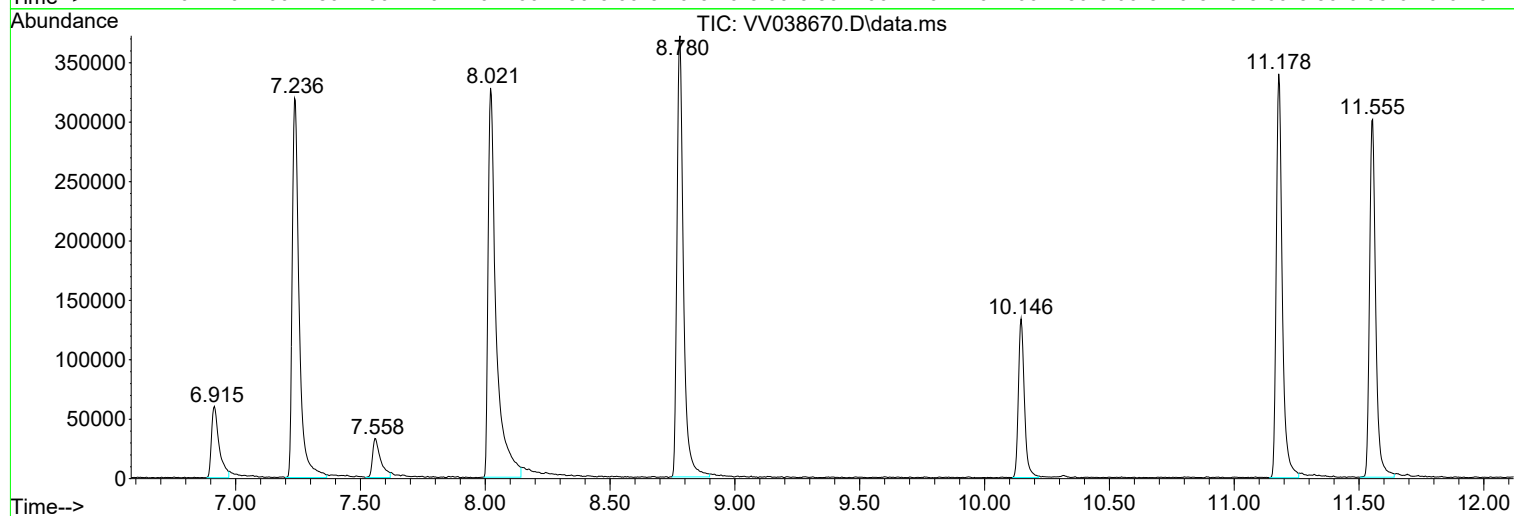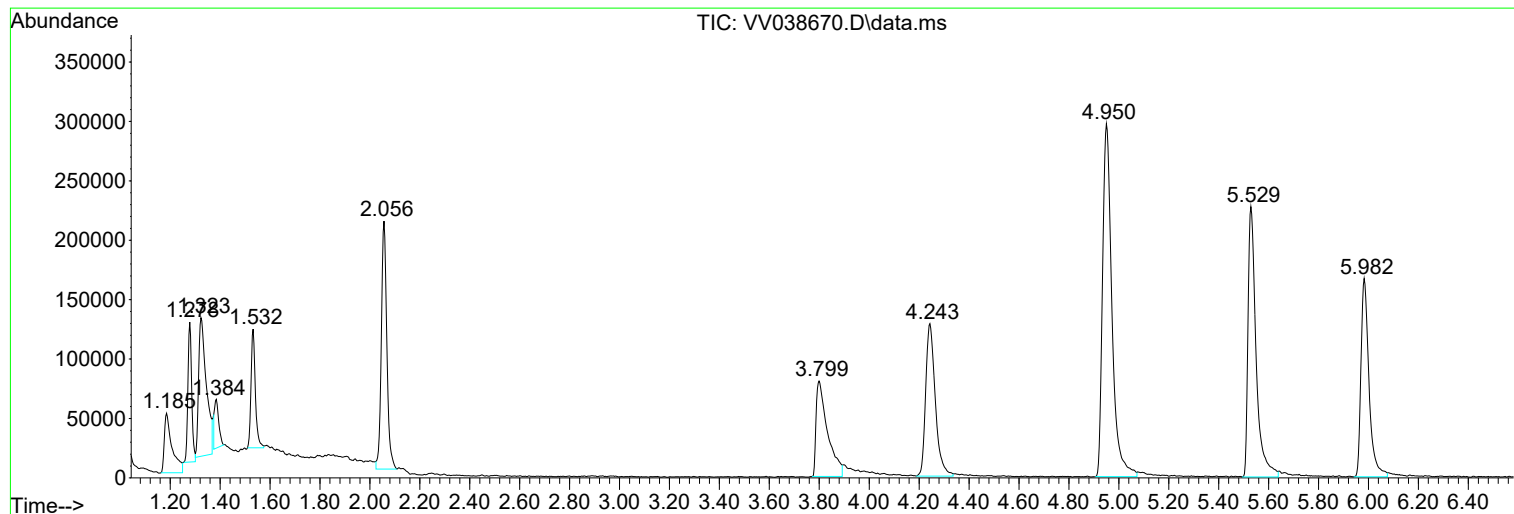

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV021025\
Data File : VV038670.D
Acq On : 10 Feb 2025 16:03
Operator : SY/MD
Sample : Q1335-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E29D0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020625WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV021025\
Data File : VV038670.D
Acq On : 10 Feb 2025 16:03
Operator : SY/MD
Sample : Q1335-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E29D0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020625WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc