
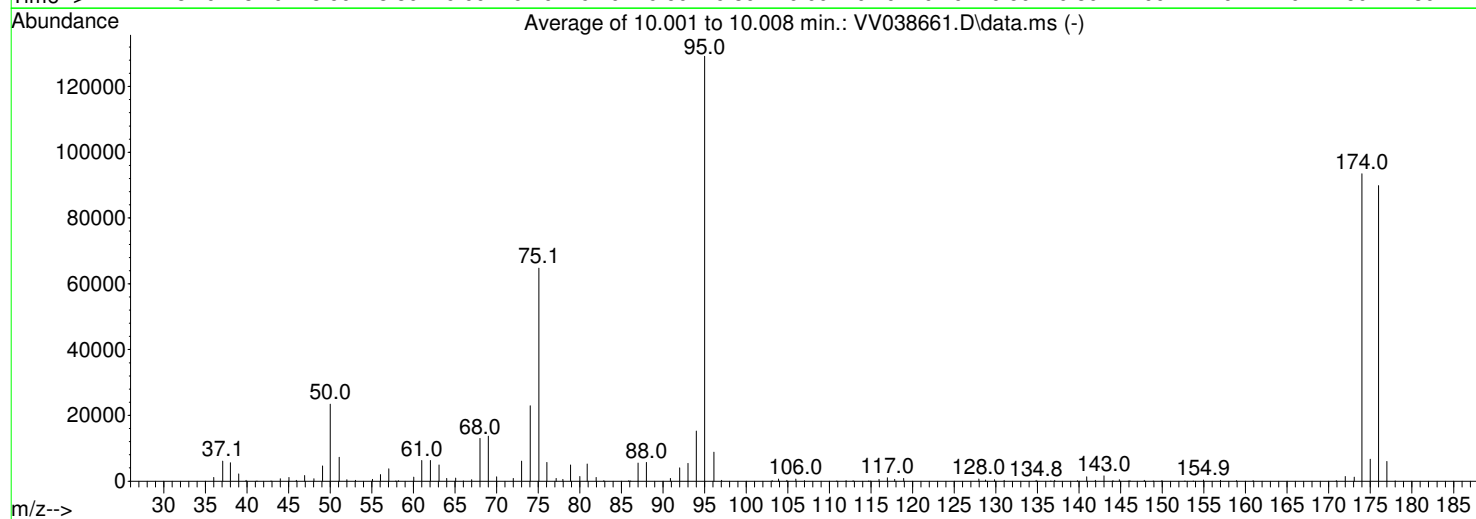


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV021025\
Data File : VV038661.D
Acq On : 10 Feb 2025 09:44
Operator : SY/MD
Sample : BFB203
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB203

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020625WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Mon Feb 17 10:31:04 2025

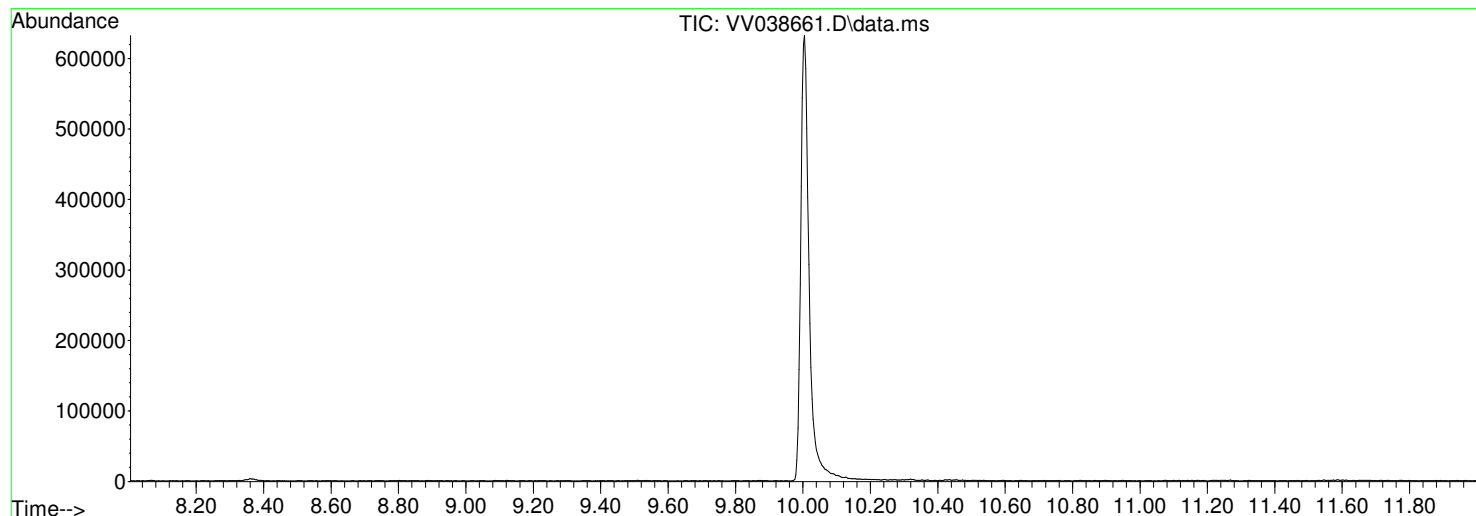

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2775

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.1	23440	PASS
75	95	30	80	50.1	64741	PASS
95	95	100	100	100.0	129187	PASS
96	95	5	9	6.8	8844	PASS
173	174	0.00	2	1.3	1206	PASS
174	95	50	120	72.4	93504	PASS
175	174	5	9	7.1	6628	PASS
176	174	95	105	96.1	89840	PASS
177	176	5	10	6.7	6013	PASS

Scan 2775 (9.963 min): VV038661.D\data.ms
BFB203

m/z	Abundance
40.00	202.0
43.90	562.0

Instrument :
MSVOA_V
ClientSampleId :
BFB203

m/z	Abundance
36.00	1136.0
37.10	6098.0
38.00	5814.0
39.00	2147.0
39.90	455.0
41.20	122.0
44.10	1331.0
45.10	1112.0
45.90	162.0
46.90	1908.0
48.10	710.0
49.10	4607.0
50.00	24232.0
51.10	7586.0
52.00	406.0
53.10	284.0
55.10	506.0
56.00	2021.0
57.10	3894.0
58.20	221.0
60.10	1221.0
61.00	6231.0
62.00	6223.0
63.10	5265.0
64.00	875.0
65.10	1007.0
67.00	373.0
68.00	13515.0
69.00	13967.0
70.00	1301.0
72.00	940.0
73.00	6215.0
74.10	22808.0
75.10	66840.0
76.10	6092.0
77.10	934.0
78.00	543.0
78.90	5168.0
80.00	1436.0
80.90	5409.0
82.00	1372.0
82.80	149.0
85.90	254.0
87.00	5613.0
88.00	6015.0
90.90	914.0
92.00	4025.0
93.00	5588.0
94.00	15516.0
95.00	131136.0
96.10	8466.0
97.00	227.0
103.00	122.0
103.80	650.0
104.90	247.0
106.00	609.0
107.00	210.0
110.90	108.0
112.00	129.0
112.90	148.0
114.70	122.0
115.90	557.0
116.90	980.0
117.80	501.0
118.90	847.0
127.90	595.0
128.70	282.0
129.80	399.0
131.00	223.0
134.90	233.0
137.10	290.0
139.80	120.0
140.90	1387.0
142.00	199.0
143.00	1632.0
144.10	157.0
144.90	400.0
145.90	160.0
147.90	192.0
148.90	106.0
149.90	150.0
152.70	132.0
155.00	326.0
157.00	272.0
158.80	119.0
160.90	146.0
170.90	177.0
172.00	1445.0
173.00	1151.0
174.00	92608.0
175.00	6670.0
176.00	89368.0

Instrument :
MSVOA_V
ClientSampleId :
BFB203

177.00

6041.0

Instrument :
MSVOA_V
ClientSampleId :
BFB203

m/z	Abundance
36.00	1103.0
37.10	6304.0
38.00	5760.0
39.00	2222.0
39.90	494.0
41.20	119.0
44.10	1310.0
45.00	1103.0
46.00	196.0
46.90	1744.0
48.10	728.0
49.10	4780.0
50.00	24176.0
51.10	7470.0
52.00	391.0
53.10	273.0
55.10	532.0
56.10	2116.0
57.00	3921.0
58.20	191.0
60.00	1209.0
61.00	6516.0
62.10	6437.0
63.10	5002.0
64.00	849.0
65.10	1006.0
67.00	455.0
68.00	13387.0
69.00	14289.0
70.00	1355.0
72.00	834.0
73.00	6273.0
74.10	23640.0
75.10	66608.0
76.10	5833.0
77.10	813.0
78.00	565.0
78.90	5027.0
80.00	1446.0
80.90	5409.0
82.00	1215.0
82.90	147.0
85.90	256.0
87.00	5666.0
88.00	5894.0
90.90	926.0
92.00	4186.0
93.00	5583.0
94.00	15647.0
95.00	133248.0
96.10	9249.0
97.10	200.0
103.10	134.0
103.90	652.0
104.90	212.0
106.00	688.0
107.00	163.0
112.00	120.0
112.80	135.0
114.70	114.0
115.90	523.0
116.90	1024.0
117.90	537.0
118.90	904.0
128.00	632.0
128.80	335.0
129.90	498.0
131.00	232.0
134.90	236.0
136.60	157.0
137.10	269.0
139.80	141.0
140.90	1386.0
141.90	227.0
143.00	1630.0
144.10	140.0
144.80	385.0
146.10	201.0
147.90	242.0
148.90	108.0
150.00	147.0
153.70	104.0
155.00	332.0
157.00	300.0
158.90	129.0
160.90	144.0
170.90	195.0
172.00	1400.0
173.10	1191.0
174.00	96560.0
175.00	6890.0
176.00	92912.0

Instrument :
MSVOA_V
ClientSampleId :
BFB203

177.006170.0

178.00109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB203

m/z	Abundance
36.00	1001.0
37.10	5758.0
38.00	5144.0
39.00	2131.0
39.90	417.0
42.90	103.0
44.10	1231.0
45.00	1026.0
46.00	255.0
47.00	1425.0
48.00	754.0
49.10	4525.0
50.00	21912.0
51.10	6651.0
52.00	402.0
53.00	205.0
55.10	467.0
56.00	1991.0
57.00	3422.0
57.90	122.0
60.00	1098.0
61.00	6216.0
62.10	6040.0
63.10	4403.0
64.00	772.0
65.10	930.0
66.00	121.0
67.00	479.0
68.00	12059.0
69.00	12885.0
70.00	1216.0
72.00	634.0
73.00	5840.0
74.00	22288.0
75.10	60776.0
76.00	5237.0
77.20	656.0
77.90	534.0
78.90	4449.0
80.00	1325.0
80.90	4810.0
81.90	916.0
83.00	158.0
86.10	203.0
87.00	5313.0
88.00	5172.0
90.90	772.0
92.00	3948.0
93.00	5150.0
94.00	14527.0
95.00	123176.0
96.10	8818.0
97.10	182.0
103.20	140.0
104.00	623.0
104.90	174.0
105.90	675.0
107.00	115.0
112.00	108.0
112.80	116.0
114.90	131.0
116.00	516.0
117.00	992.0
117.90	536.0
118.90	817.0
128.00	602.0
128.80	287.0
129.90	529.0
131.00	238.0
134.80	252.0
137.00	193.0
139.80	119.0
140.90	1269.0
141.90	220.0
143.00	1497.0
144.00	113.0
144.90	423.0
146.10	194.0
147.80	305.0
150.00	145.0
154.90	271.0
157.00	312.0
159.00	137.0
160.90	117.0
170.90	179.0
172.00	1355.0
173.10	1275.0
174.00	91344.0
175.00	6325.0
176.00	87240.0
177.00	5827.0
178.00	121.0

Instrument :
MSVOA_V
ClientSampleId :
BFB203