


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV021120\
 Data File : VV014553.D
 Acq On : 11 Feb 2020 09:18
 Operator : SY/MD
 Sample : BFB88
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB88

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM020120WMA.M
 Title : VOC Analysis
 Last Update : Wed Feb 12 03:16:31 2020

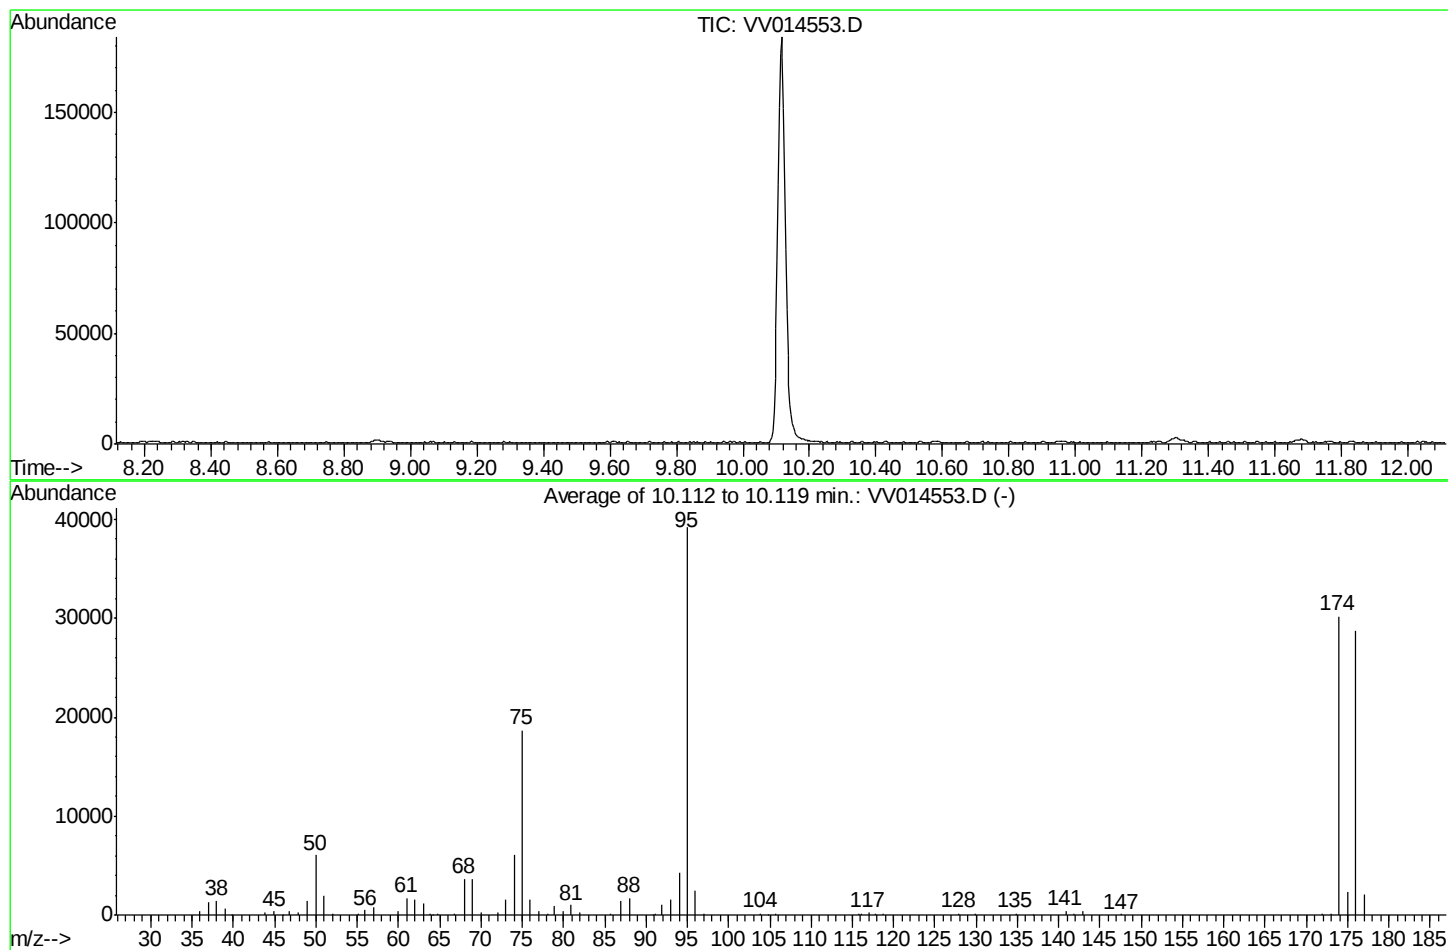

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.5	6081	PASS
75	95	30	80	47.7	18706	PASS
95	95	100	100	100.0	39205	PASS
96	95	5	9	6.3	2489	PASS
173	174	0.00	2	0.5	164	PASS
174	95	50	120	77.0	30184	PASS
175	174	5	9	7.8	2348	PASS
176	174	95	101	95.0	28682	PASS
177	176	5	9	7.2	2074	PASS

m/z	Abundance
35.90	316.0
37.00	1291.0
38.00	1293.0
38.90	531.0
39.80	237.0
44.00	469.0
45.00	375.0
46.90	376.0
47.80	290.0
48.90	1317.0
50.00	5810.0
51.00	1871.0
52.10	131.0
55.10	159.0
56.00	466.0
57.10	781.0
60.00	361.0
61.00	1784.0
62.00	1619.0
63.00	1029.0
63.80	114.0
66.80	148.0
68.00	3672.0
69.00	3638.0
70.00	243.0
72.00	241.0
73.00	1469.0
74.00	5973.0
75.00	18112.0
76.00	1576.0
77.00	312.0
78.00	134.0
78.80	1025.0
79.90	315.0
80.90	968.0
82.00	171.0
85.70	180.0
86.90	1292.0
87.90	1614.0
91.00	152.0
91.90	1077.0
93.00	1544.0
94.00	4182.0
95.00	38600.0
96.00	2421.0
97.10	124.0
103.80	187.0
105.70	153.0
115.70	132.0
116.90	238.0
117.80	110.0
118.70	180.0
127.90	165.0
130.00	133.0
134.80	123.0
140.90	423.0
141.80	124.0
142.90	385.0
171.90	157.0
173.90	30040.0
175.00	2369.0
175.90	28248.0
176.90	1997.0

Instrument :
MSVOA_V
ClientSampleId :
BFB88

m/z	Abundance
35.90	350.0
37.00	1327.0
38.00	1515.0
38.90	634.0
39.80	242.0
44.00	527.0
45.00	387.0
46.80	445.0
47.80	271.0
48.90	1413.0
50.00	6240.0
51.00	2054.0
52.10	122.0
55.10	190.0
55.90	508.0
57.10	747.0
60.00	405.0
61.00	1821.0
62.00	1593.0
63.00	1163.0
63.80	131.0
64.70	115.0
66.80	128.0
68.00	3781.0
69.00	3802.0
70.00	242.0
72.00	254.0
73.00	1619.0
74.00	6290.0
75.00	19272.0
76.00	1614.0
77.00	356.0
78.10	147.0
78.90	972.0
80.00	386.0
80.90	1003.0
81.90	209.0
85.70	151.0
86.90	1392.0
88.00	1807.0
91.10	151.0
91.90	1129.0
93.00	1561.0
94.00	4312.0
95.00	40456.0
96.00	2555.0
97.10	107.0
103.80	171.0
105.70	142.0
115.70	107.0
116.10	134.0
117.00	245.0
117.80	117.0
118.70	188.0
127.90	166.0
130.00	117.0
134.80	149.0
140.80	456.0
141.90	123.0
143.00	370.0
147.60	111.0
171.90	158.0
173.90	31144.0
175.00	2488.0
175.90	29720.0
177.00	2141.0

Instrument :
MSVOA_V
ClientSampleId :
BFB88

m/z	Abundance
35.90	324.0
37.00	1324.0
38.00	1611.0
39.00	635.0
39.80	270.0
43.90	541.0
44.90	388.0
46.00	110.0
46.80	435.0
47.80	260.0
48.90	1398.0
50.00	6193.0
51.00	1923.0
52.10	109.0
55.10	175.0
55.90	496.0
57.00	708.0
60.00	371.0
61.00	1628.0
62.00	1443.0
63.00	1163.0
64.10	143.0
64.70	125.0
66.90	118.0
68.00	3606.0
69.00	3597.0
70.00	202.0
72.00	253.0
73.00	1663.0
74.00	5899.0
75.00	18736.0
76.00	1500.0
76.90	316.0
78.10	159.0
78.90	880.0
80.00	386.0
80.90	965.0
81.90	231.0
85.70	109.0
86.90	1449.0
88.00	1764.0
90.80	161.0
92.00	1035.0
93.00	1451.0
94.00	4165.0
95.00	38560.0
96.00	2491.0
97.00	111.0
103.90	158.0
104.70	122.0
105.90	137.0
116.10	147.0
117.00	217.0
117.80	122.0
118.90	163.0
127.90	124.0
129.90	122.0
134.80	149.0
136.90	103.0
140.80	449.0
141.90	105.0
142.90	300.0
147.60	111.0
171.90	144.0
173.00	494.0
173.90	29368.0
174.90	2188.0
175.90	28080.0
177.00	2085.0

Instrument :
MSVOA_V
ClientSampleId :
BFB88

Scan 2795 (10.077 min): VV014553.D
BFB88

m/z	Abundance
37.30	104.0
39.80	204.0
43.90	277.0
65.80	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB88