

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021121\
Data File : VW020297.D
Acq On : 11 Feb 2021 12:09
Operator : SY/MD
Sample : M1375-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BJ5

Manual Integrations
APPROVED

MMDadoda
2/12/2021 2:02:10 PM

Quant Time: Feb 12 00:26:55 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 12 00:25:49 2021
Response via : Initial Calibration

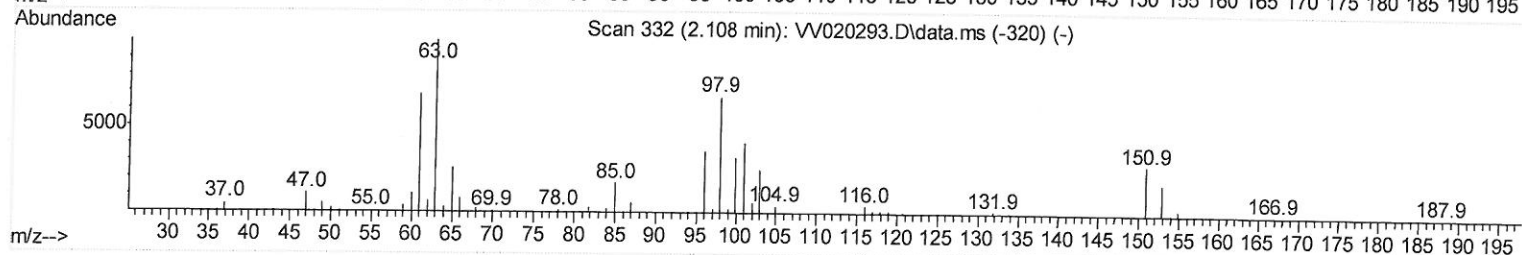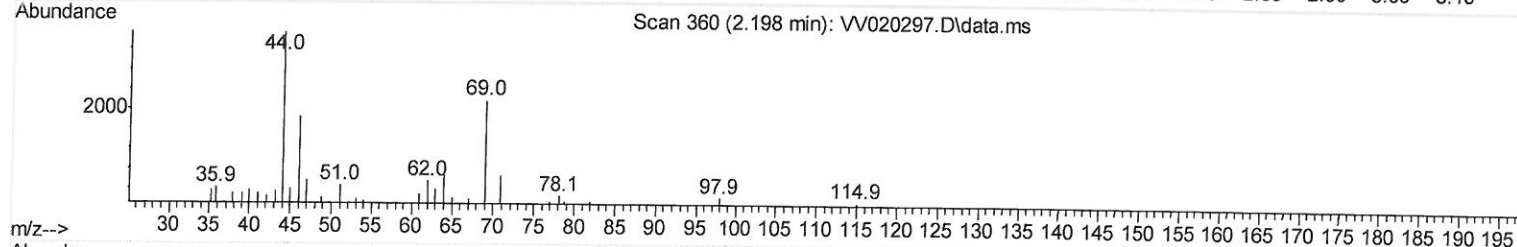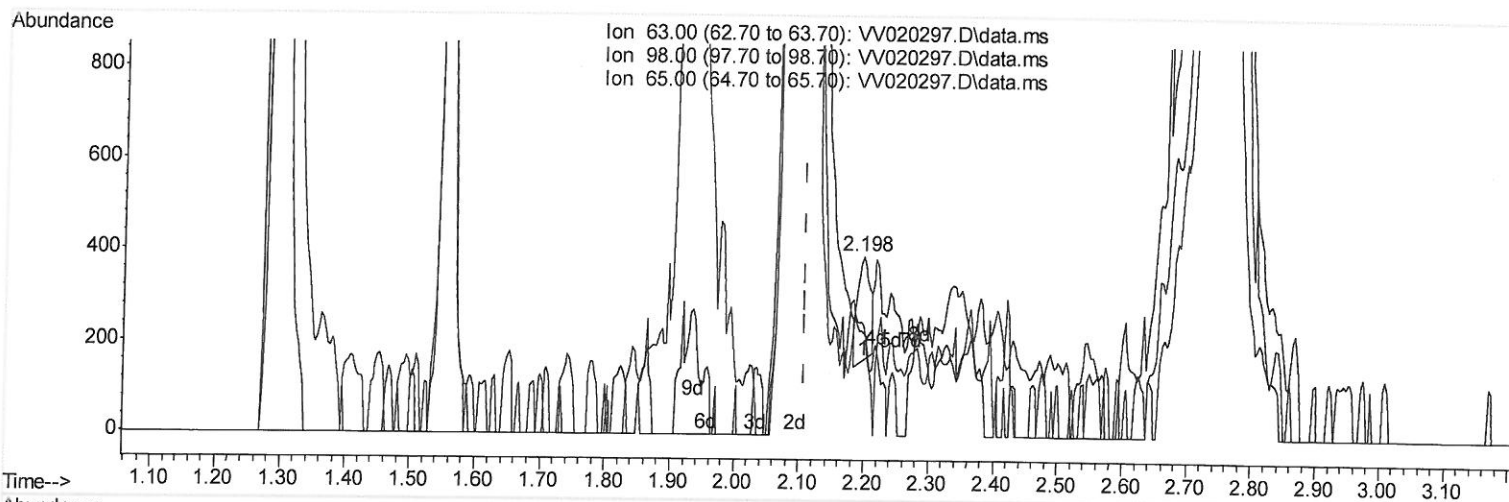

TIC: VW020297.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.198min (+ 0.090) 0.05 ug/L

response 303

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	66.80	55.78
65.00	23.90	28.38
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021121\
Data File : VV020297.D
Acq On : 11 Feb 2021 12:09
Operator : SY/MD
Sample : M1375-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BJ5

Manual Integrations
APPROVED

MMDadoda
2/12/2021 2:02:10 PM

Quant Time: Feb 12 00:26:55 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 12 00:25:49 2021
Response via : Initial Calibration

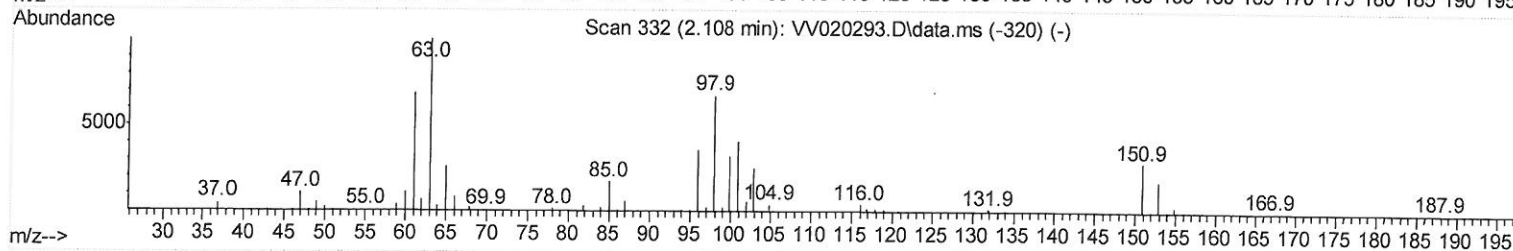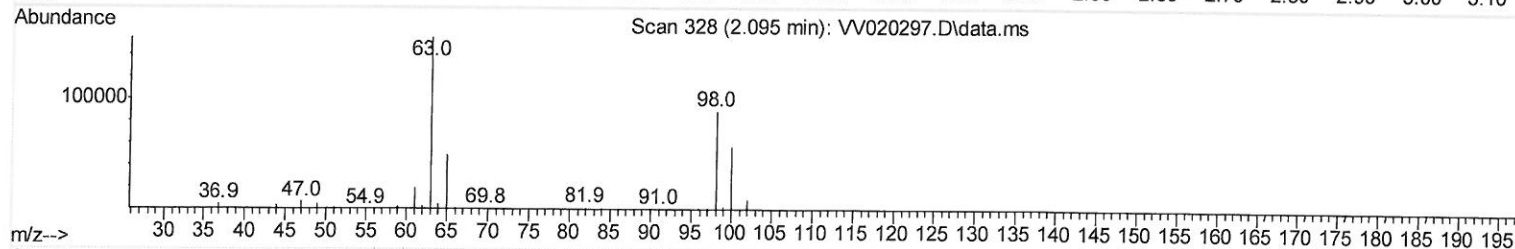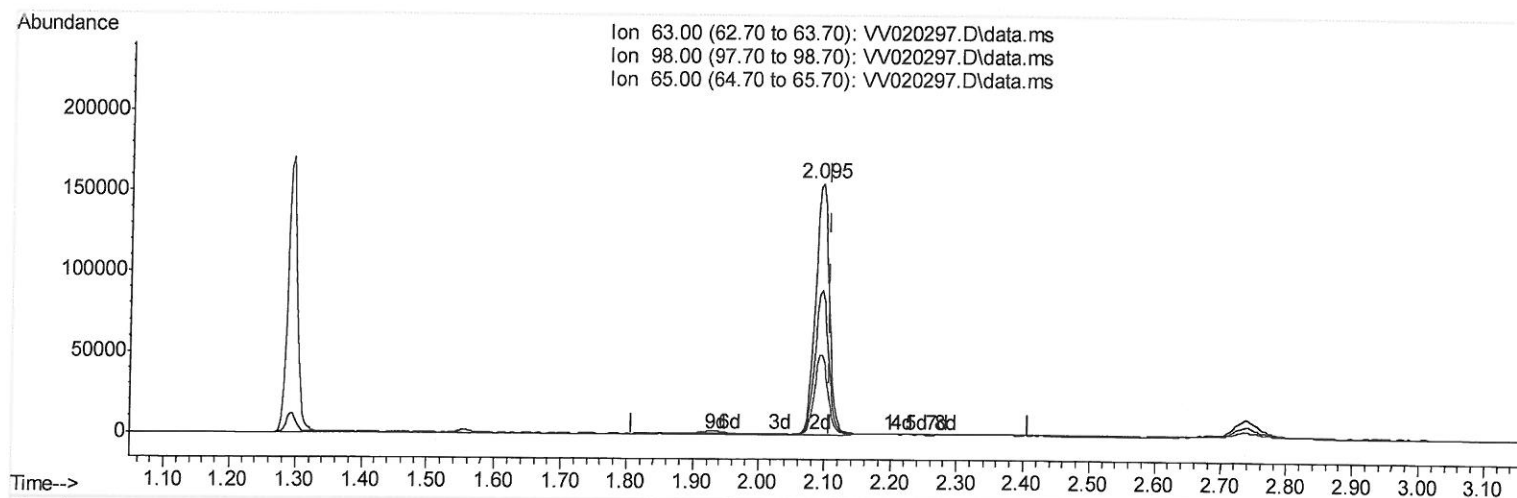

TIC: VV020297.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.095min (-0.013) 37.48 ug/L m

response 224980

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	66.80	0.08#
65.00	23.90	0.04#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021121\
Data File : VW020297.D
Acq On : 11 Feb 2021 12:09
Operator : SY/MD
Sample : M1375-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BJ5

Manual Integrations
APPROVED

MMDadoda
2/12/2021 2:02:10 PM

Quant Time: Feb 12 00:26:55 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 12 00:25:49 2021
Response via : Initial Calibration

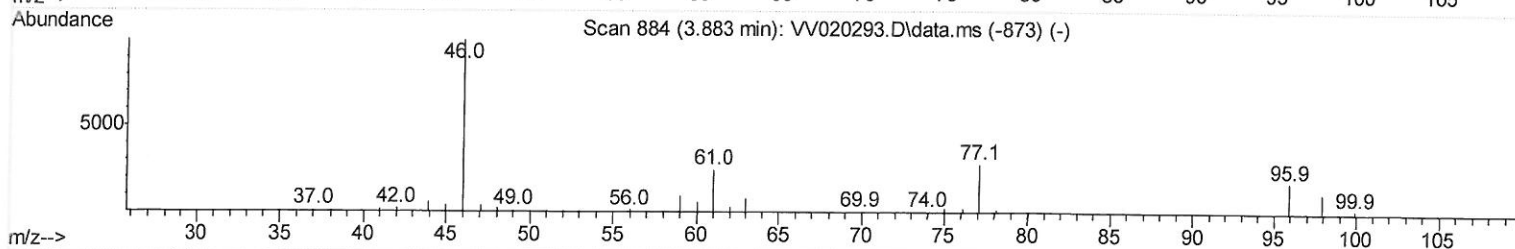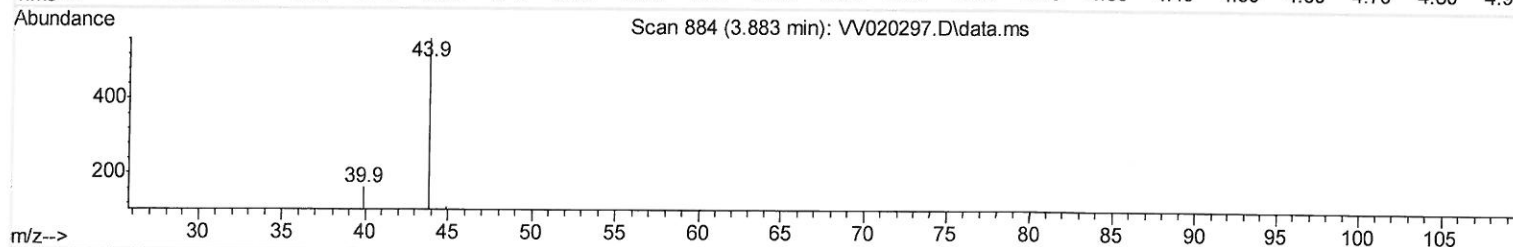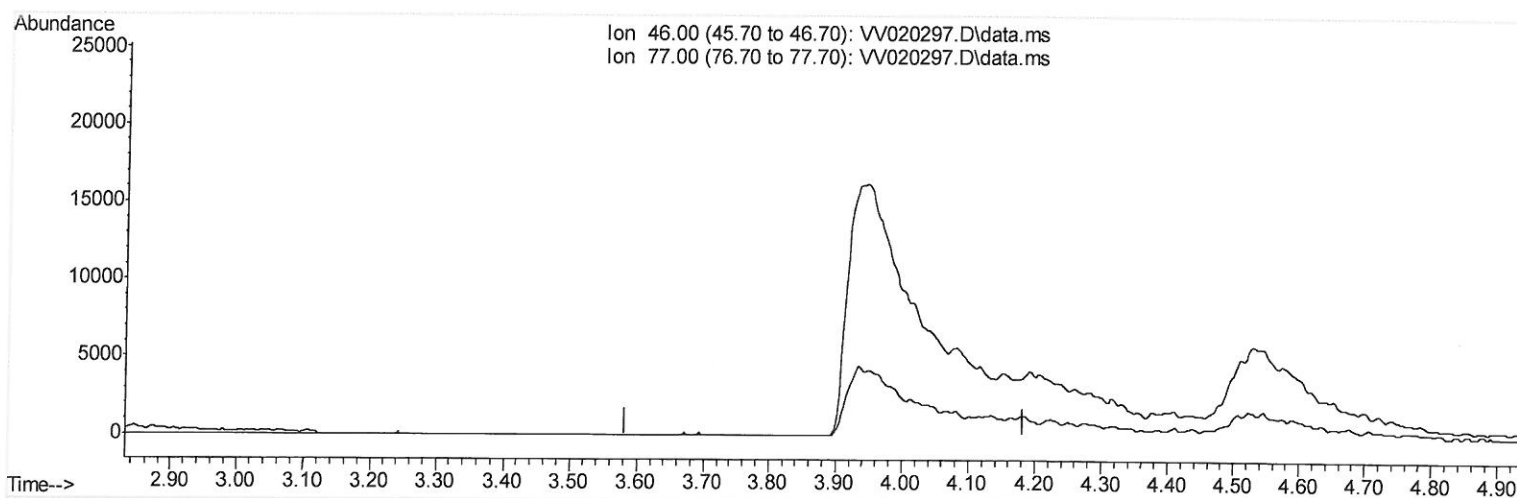

TIC: VW020297.D\data.ms

(21) 2-Butanone-d5 (S)

3.883min (-3.883) 0.00 ug/L

response 0

Ion	Exp%	Act%
46.00	100.00	0.00
77.00	22.90	0.00#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021121\
Data File : VV020297.D
Acq On : 11 Feb 2021 12:09
Operator : SY/MD
Sample : M1375-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BJ5

Manual Integrations
APPROVED

MMDadoda
2/12/2021 2:02:10 PM

Quant Time: Feb 12 00:26:55 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 12 00:25:49 2021
Response via : Initial Calibration

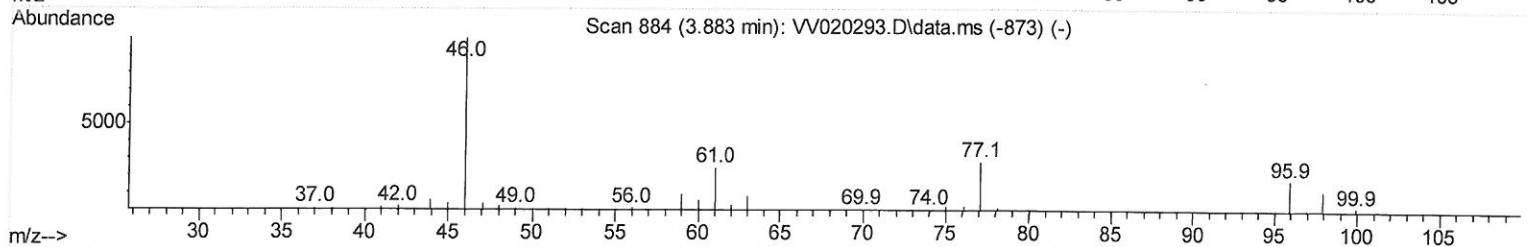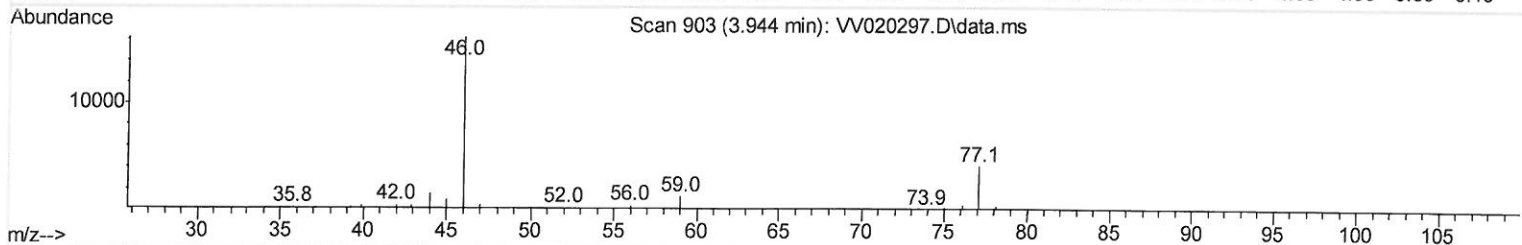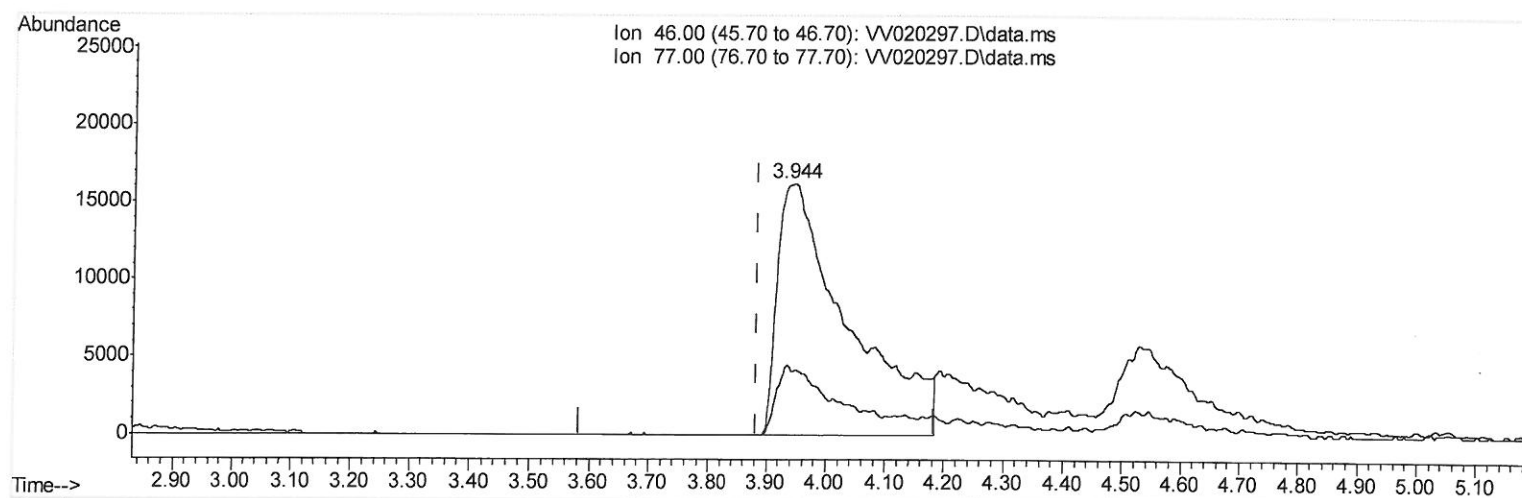

TIC: VV020297.D\data.ms

(21) 2-Butanone-d5 (S)

3.944min (+ 0.061) 74.77 ug/L m

response 132655

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	22.90	0.00#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\V021121\
 Data File : V020297.D
 Acq On : 11 Feb 2021 12:09
 Operator : SY/MD
 Sample : M1375-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BJ5

Manual Integrations
 APPROVED

MMDadoda
 2/12/2021 2:02:10 PM

Quant Time: Feb 12 00:26:55 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Feb 12 00:25:49 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	435550	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	442454	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.259	152	234776	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.294	65	170075	53.56	ug/L	-0.01
Spiked Amount 50.000	Range 60 - 135		Recovery = 107.12%			
7) Chloroethane-d5	1.555	69	136494	52.39	ug/L	-0.01
Spiked Amount 50.000	Range 70 - 130		Recovery = 104.78%			
11) 1,1-Dichloroethene-d2	2.095	63	224980m	37.48	ug/L	-0.01
Spiked Amount 50.000	Range 60 - 125		Recovery = 74.96%			
21) 2-Butanone-d5	3.944	46	132655m	74.77	ug/L	0.06
Spiked Amount 100.000	Range 40 - 130		Recovery = 74.77%			
24) Chloroform-d	4.342	84	259694	45.96	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 91.92%			
26) 1,2-Dichloroethane-d4	5.027	65	172238	48.08	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 96.16%			
32) Benzene-d6	5.043	84	545729	47.61	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 95.22%			
36) 1,2-Dichloropropane-d6	6.066	67	162821	47.58	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 95.16%			
41) Toluene-d8	7.317	98	503701	46.76	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 93.52%			
43) trans-1,3-Dichloroprop...	7.622	79	74900	42.94	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 85.88%			
47) 2-Hexanone-d5	8.098	63	120413	84.57	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 84.57%			
57) 1,1,2,2-Tetrachloroeth...	10.223	84	238461	48.53	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 97.06%			
64) 1,2-Dichlorobenzene-d4	11.632	152	239263	53.86	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 107.72%			
Target Compounds						Qvalue
25) Chloroform	4.371	83	11118	2.09	ug/L	84

(#) = qualifier out of range (m) = manual integration (+) = signals summed

02/15/2024

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021121\
Data File : VW020297.D
Acq On : 11 Feb 2021 12:09
Operator : SY/MD
Sample : M1375-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BJ5

Manual Integrations
APPROVED

MMDadoda
2/12/2021 2:02:10 PM

Quant Time: Feb 12 00:26:55 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 12 00:25:49 2021
Response via : Initial Calibration

