

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021121\
 Data File : VW020298.D
 Acq On : 11 Feb 2021 14:53
 Operator : SY/MD
 Sample : M1375-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BJ2

Quant Time: Feb 12 00:27:10 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Feb 12 00:25:49 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	606099	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	611998	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	295829	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	173315	39.22	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	78.44%		
7) Chloroethane-d5	1.568	69	157330	43.39	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	86.78%		
11) 1,1-Dichloroethene-d2	2.108	63	266982	31.96	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	63.92%		
21) 2-Butanone-d5	3.876	46	261350	105.86	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	105.86%		
24) Chloroform-d	4.349	84	316180	40.21	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	80.42%		
26) 1,2-Dichloroethane-d4	5.030	65	239880	48.12	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.24%		
32) Benzene-d6	5.050	84	700463	44.18	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.36%		
36) 1,2-Dichloropropane-d6	6.069	67	218972	46.26	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	92.52%		
41) Toluene-d8	7.317	98	663135	44.50	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	89.00%		
43) trans-1,3-Dichloroprop...	7.622	79	102075	42.30	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	84.60%		
47) 2-Hexanone-d5	8.088	63	207095	105.16	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	105.16%		
57) 1,1,2,2-Tetrachloroeth...	10.220	84	298851	43.97	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	87.94%		
64) 1,2-Dichlorobenzene-d4	11.631	152	272610	48.70	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	97.40%		
Target Compounds					Qvalue	
13) Acetone	2.169	43	19595	11.24	ug/L	87
25) Chloroform	4.375	83	37204	5.02	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021121\
Data File : VV020298.D
Acq On : 11 Feb 2021 14:53
Operator : SY/MD
Sample : M1375-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BJ2

Quant Time: Feb 12 00:27:10 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 12 00:25:49 2021
Response via : Initial Calibration




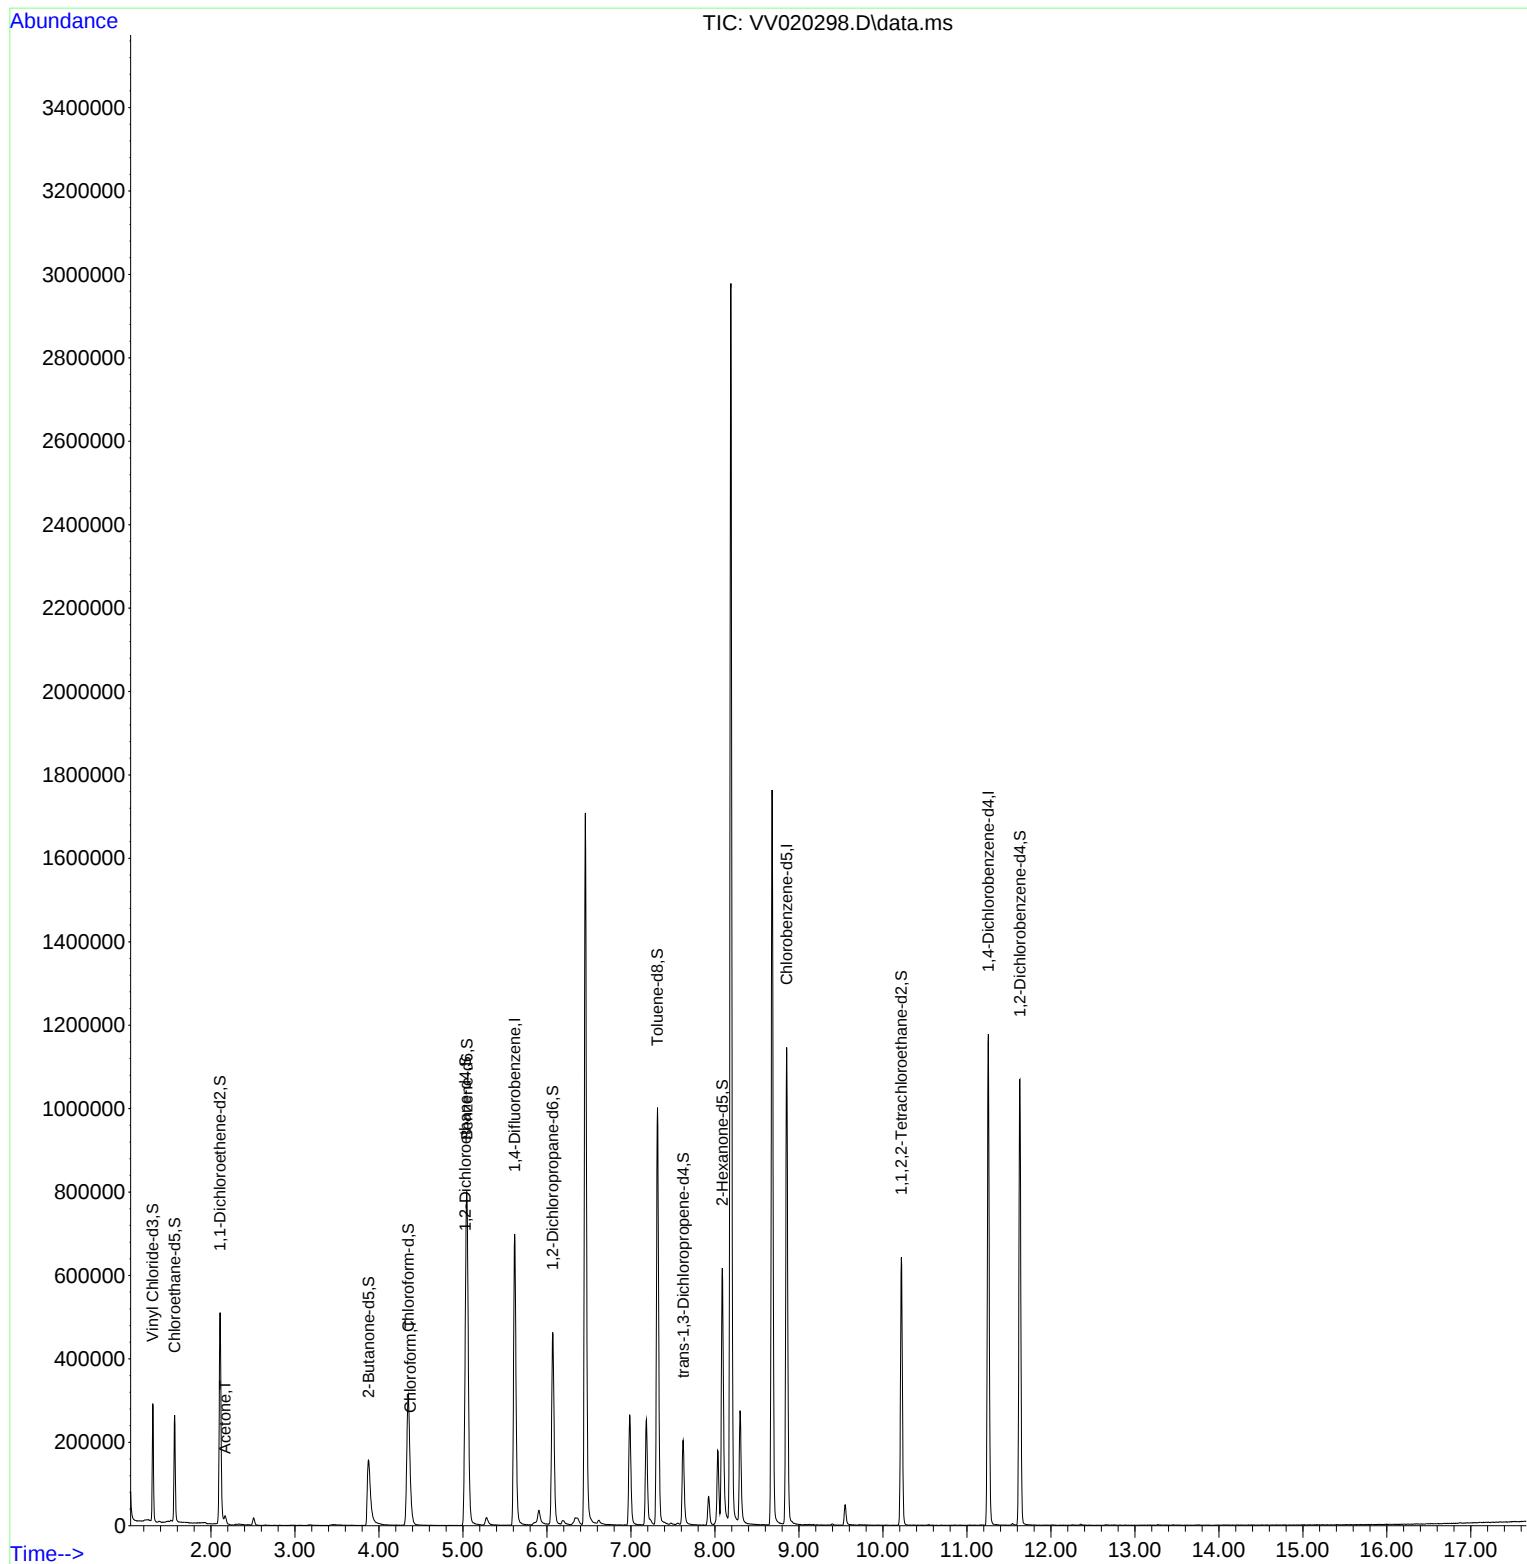


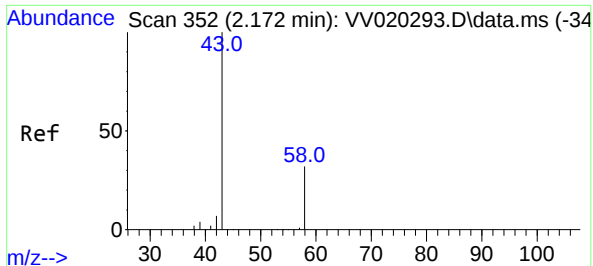

#13
Acetone
Concen: 11.24 ug/L
RT: 2.169 min Scan# 351
Delta R.T. -0.003 min
Lab File: VV020298.D
Acq: 11 Feb 2021 14:53

Instrument :
MSVOA_V
ClientSampled :
C0BJ2

Tgt Ion: 43 Resp: 19595
Ion Ratio Lower Upper
43 100
58 37.0 0.0 60.2

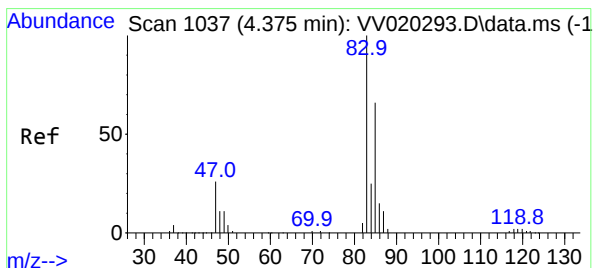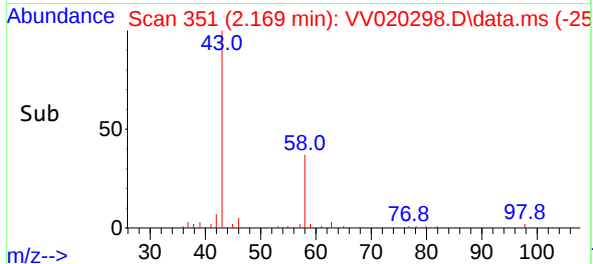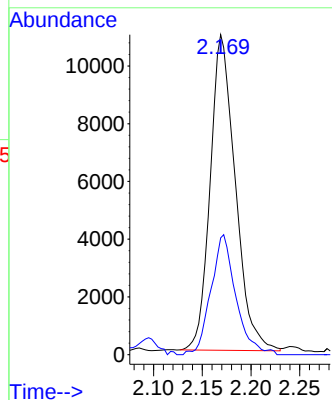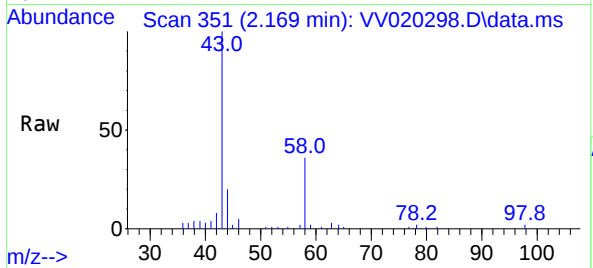

#25
Chloroform
Concen: 5.02 ug/L
RT: 4.375 min Scan# 1037
Delta R.T. -0.000 min
Lab File: VV020298.D
Acq: 11 Feb 2021 14:53

Tgt Ion: 83 Resp: 37204
Ion Ratio Lower Upper
83 100
85 66.2 44.2 82.2

