

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021121\
 Data File : VV020301.D
 Acq On : 11 Feb 2021 16:29
 Operator : SY/MD
 Sample : PB134573TB
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VLEB01

Quant Time: Feb 12 00:27:58 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Feb 12 00:25:49 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	600661	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	599651	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	283980	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	165498	37.79	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	75.58%
7) Chloroethane-d5	1.568	69	150576	41.91	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	83.82%
11) 1,1-Dichloroethene-d2	2.111	63	257430	31.10	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	62.20%
21) 2-Butanone-d5	3.883	46	247103	101.00	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	101.00%
24) Chloroform-d	4.352	84	307238	39.42	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	78.84%
26) 1,2-Dichloroethane-d4	5.034	65	222647	45.07	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.14%
32) Benzene-d6	5.053	84	659865	42.47	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.94%
36) 1,2-Dichloropropane-d6	6.072	67	208577	44.97	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	89.94%
41) Toluene-d8	7.320	98	613470	42.02	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	84.04%
43) trans-1,3-Dichloroprop...	7.625	79	98786	41.78	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.56%
47) 2-Hexanone-d5	8.091	63	200269	103.79	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	103.79%
57) 1,1,2,2-Tetrachloroeth...	10.223	84	285314	42.84	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	85.68%
64) 1,2-Dichlorobenzene-d4	11.631	152	253618	47.20	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.40%
Target Compounds						
13) Acetone	2.175	43	16239	9.40	ug/L	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021121\
Data File : VV020301.D
Acq On : 11 Feb 2021 16:29
Operator : SY/MD
Sample : PB134573TB
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VLEB01


Quant Time: Feb 12 00:27:58 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 12 00:25:49 2021
Response via : Initial Calibration

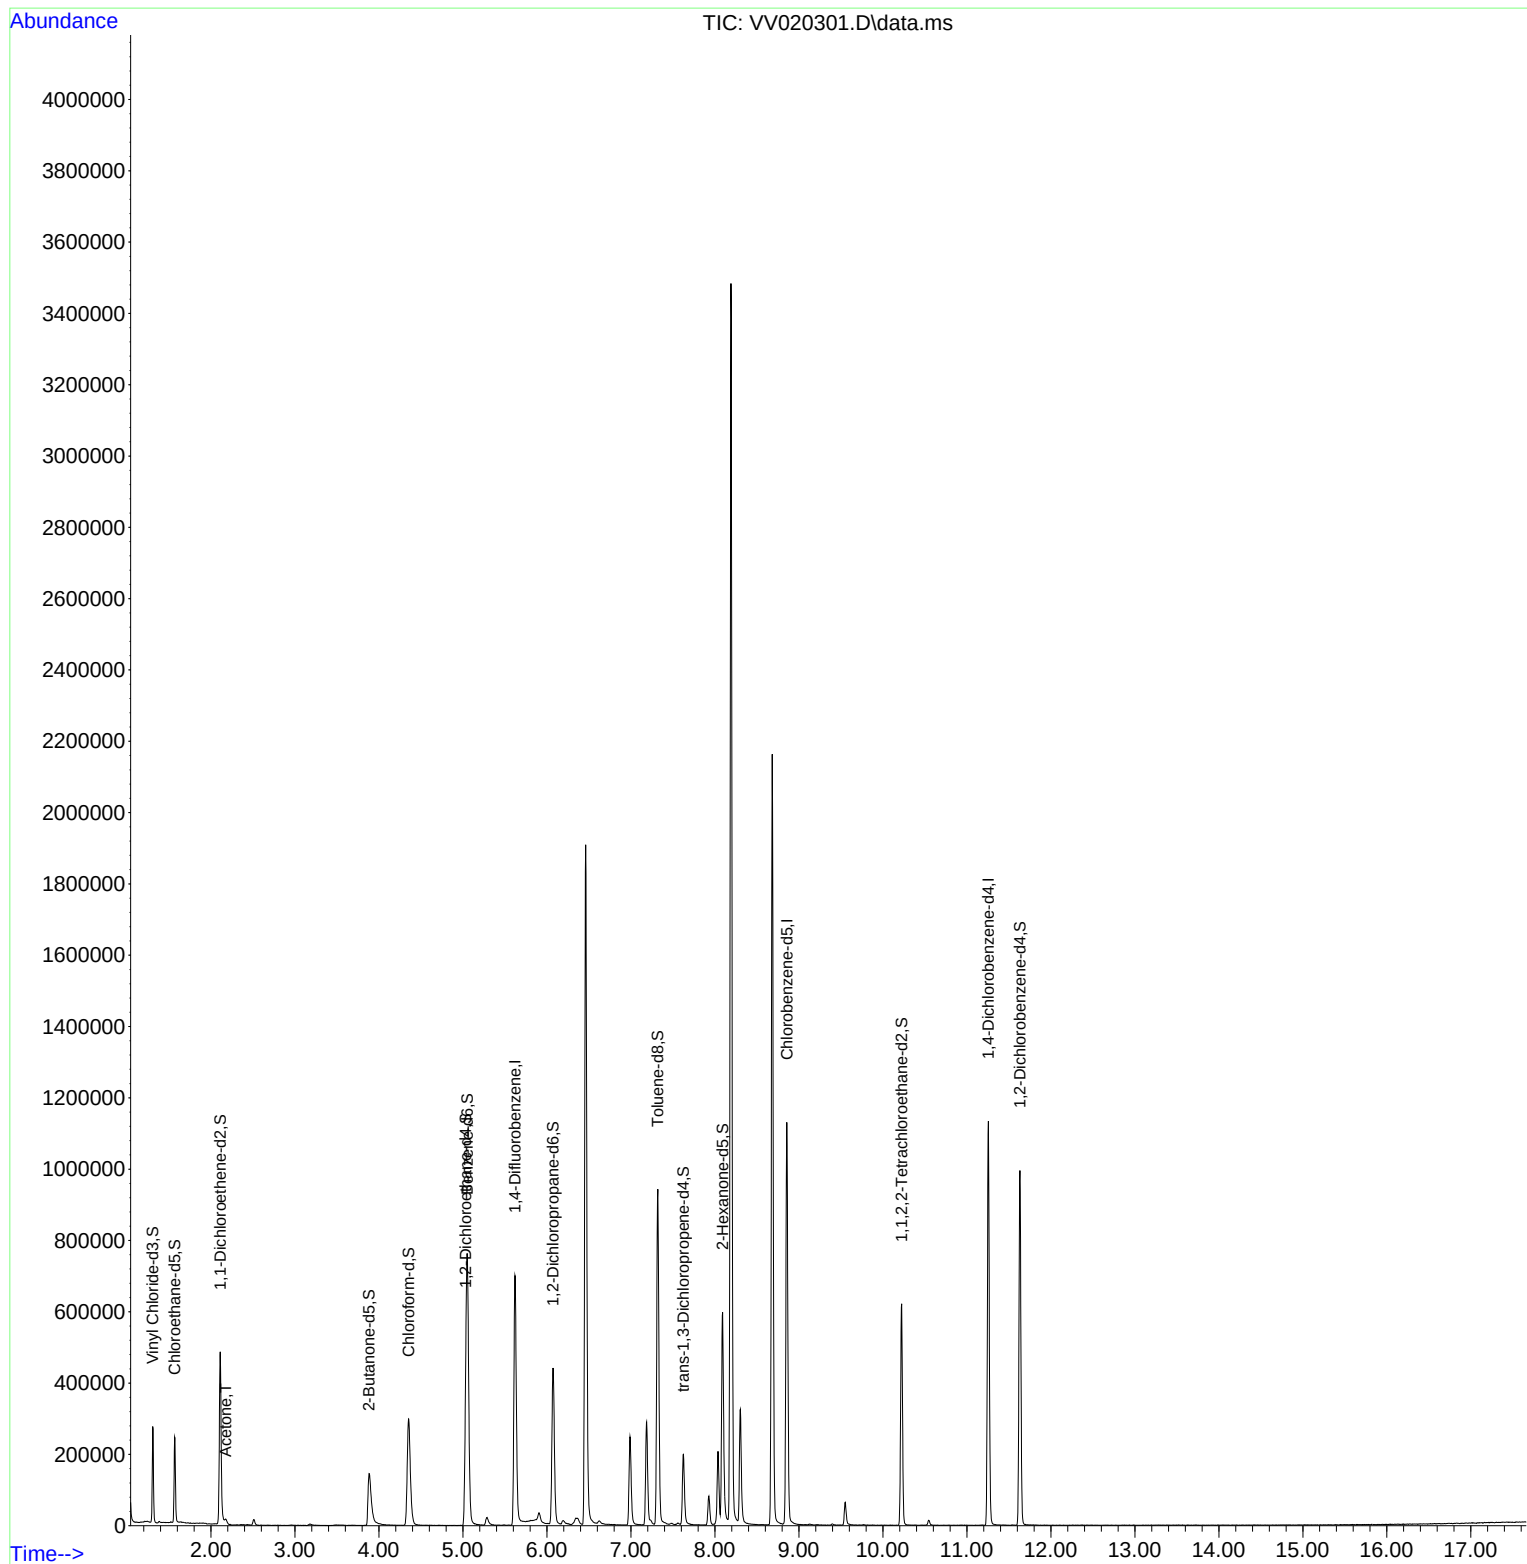

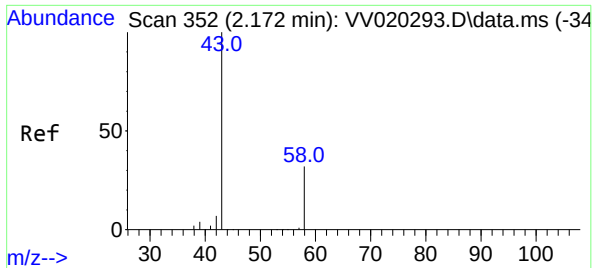

#13
 Acetone
 Concen: 9.40 ug/L
 RT: 2.175 min Scan# 353
 Delta R.T. 0.003 min
 Lab File: VV020301.D
 Acq: 11 Feb 2021 16:29

Instrument :
 MSVOA_V
 ClientSampleId :
 VLEB01

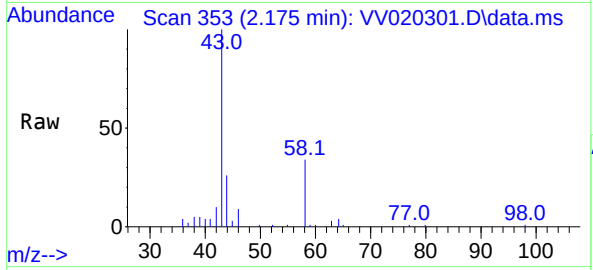

Tgt Ion: 43 Resp: 16239

Ion	Ratio	Lower	Upper
43	100		
58	35.1	0.0	60.2

