

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021121\
 Data File : VW020302.D
 Acq On : 11 Feb 2021 16:52
 Operator : SY/MD
 Sample : VIBLK02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK02

Quant Time: Feb 12 00:28:13 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Feb 12 00:25:49 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	582072	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	561053	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.256	152	273641	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	168194	39.63	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	79.26%	
7) Chloroethane-d5	1.568	69	153472	44.08	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	88.16%	
11) 1,1-Dichloroethene-d2	2.108	63	259197	32.31	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	64.62%	
21) 2-Butanone-d5	3.883	46	222695	93.93	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	93.93%	
24) Chloroform-d	4.352	84	317136	41.99	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	83.98%	
26) 1,2-Dichloroethane-d4	5.034	65	219550	45.86	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	91.72%	
32) Benzene-d6	5.053	84	655020	45.06	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	90.12%	
36) 1,2-Dichloropropane-d6	6.072	67	208272	47.99	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	95.98%	
41) Toluene-d8	7.320	98	599512	43.89	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	87.78%	
43) trans-1,3-Dichloroprop...	7.625	79	92760	41.93	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	83.86%	
47) 2-Hexanone-d5	8.092	63	162986	90.28	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	90.28%	
57) 1,1,2,2-Tetrachloroeth...	10.223	84	281572	45.19	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	90.38%	
64) 1,2-Dichlorobenzene-d4	11.632	152	246871	47.68	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	95.36%	
Target Compounds						
25) Chloroform	4.381	83	17705	2.49	ug/L	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021121\
Data File : VV020302.D
Acq On : 11 Feb 2021 16:52
Operator : SY/MD
Sample : VIBLK02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK02

Quant Time: Feb 12 00:28:13 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 12 00:25:49 2021
Response via : Initial Calibration

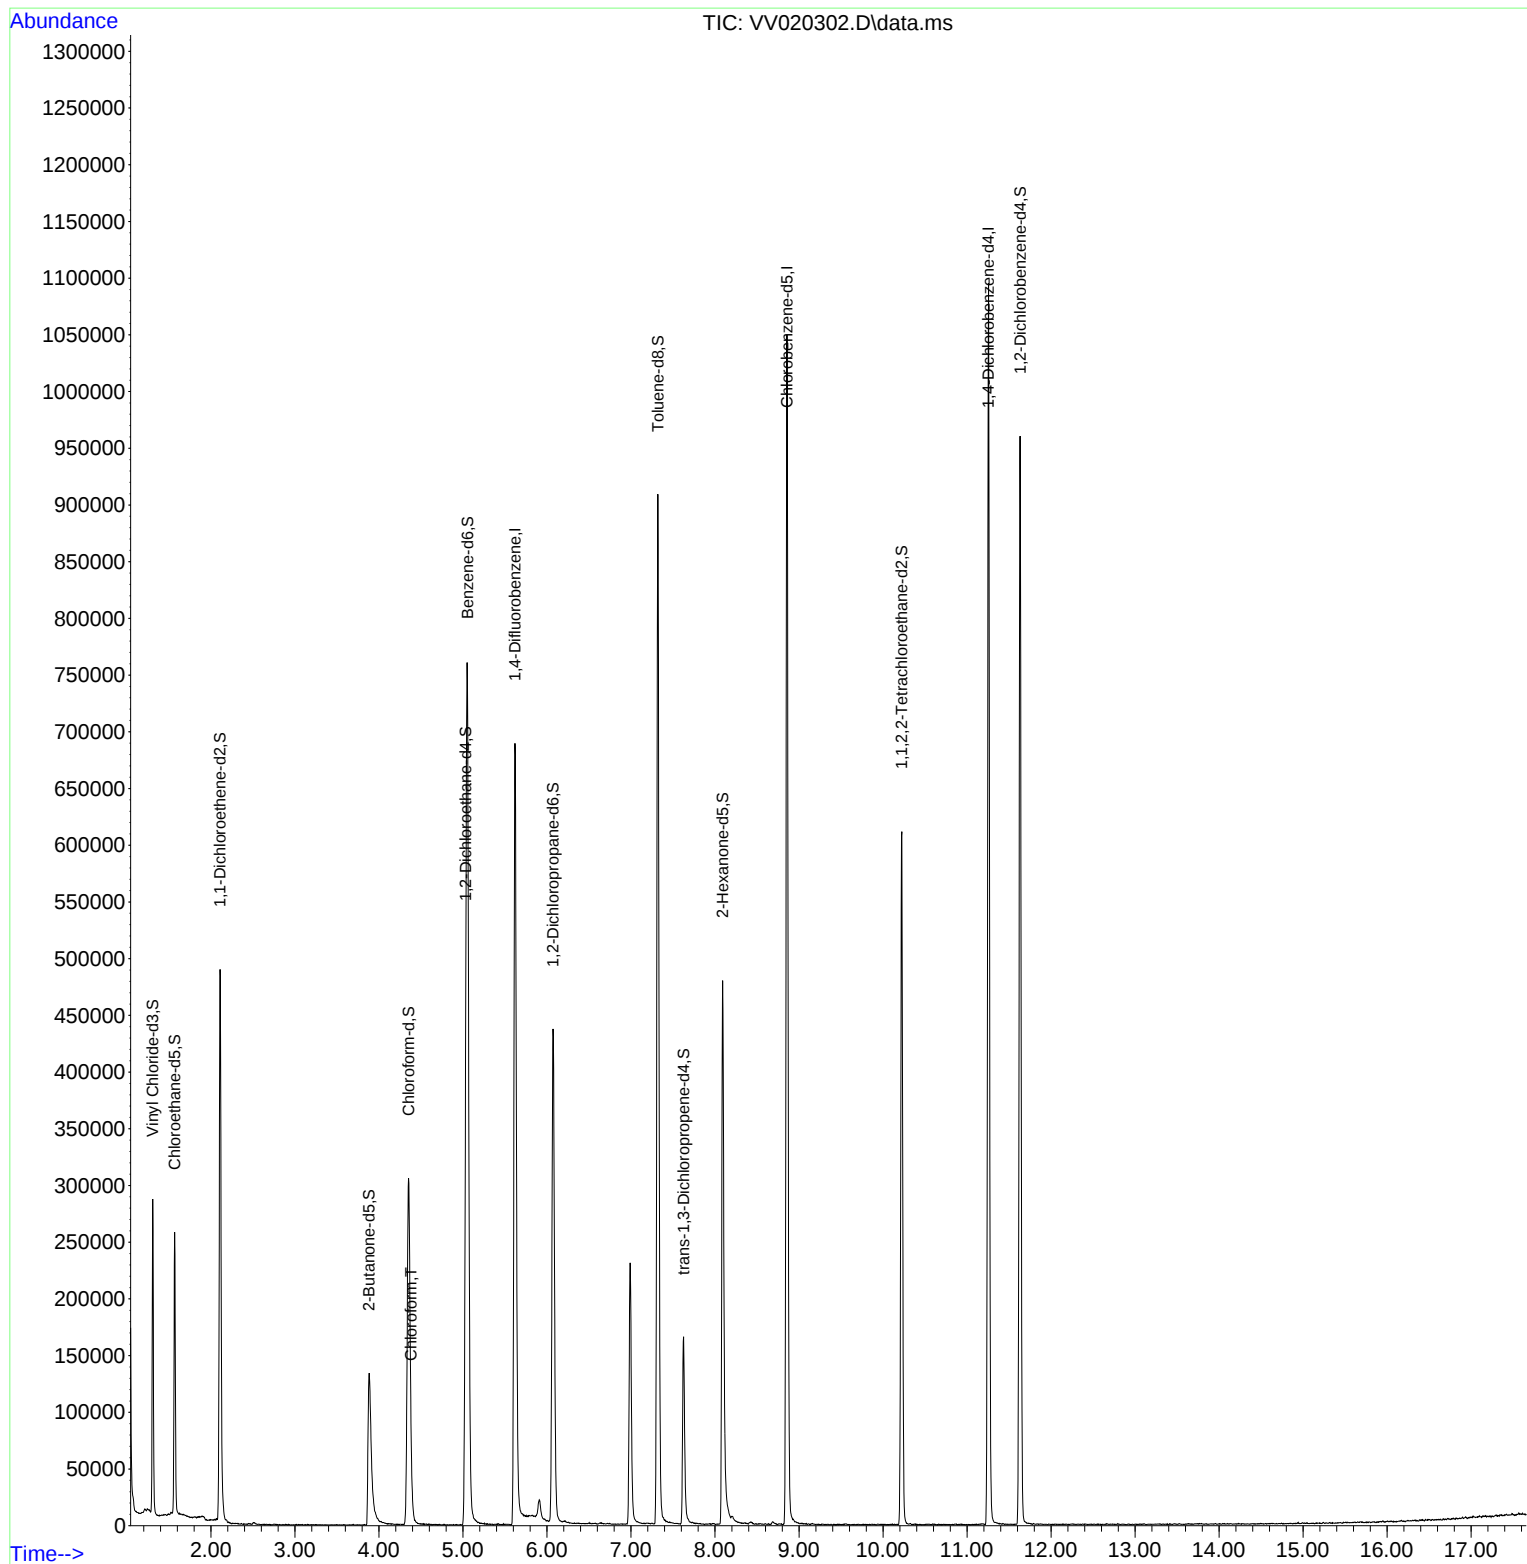

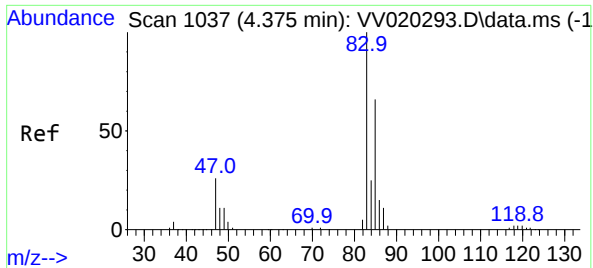

#25
 Chloroform
 Concen: 2.49 ug/L
 RT: 4.381 min Scan# 1039
 Delta R.T. 0.007 min
 Lab File: VV020302.D
 Acq: 11 Feb 2021 16:52

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK02

Tgt Ion:	83	Resp:	17705
Ion	Ratio	Lower	Upper
83	100		
85	68.3	44.2	82.2

