

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021121\
 Data File : VV020297.D
 Acq On : 11 Feb 2021 12:09
 Operator : SY/MD
 Sample : M1375-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BJ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

Signal : TIC: VV020297.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.294	73	79	97	rVB	286563	289233	18.19%	2.261%
2	1.555	154	160	172	rVB	212807	233514	14.69%	1.825%
3	2.095	319	328	343	rVB	414421	588020	36.98%	4.596%
4	3.127	647	649	651	rBV	545	259	0.02%	0.002%
5	3.195	668	670	672	rBV2	640	331	0.02%	0.003%
6	3.323	708	710	712	rVB	259	78	0.00%	0.001%
7	3.445	746	748	749	rBV2	281	84	0.01%	0.001%
8	3.542	776	778	781	rBV	280	179	0.01%	0.001%
9	3.593	793	794	795	rBV	108	28	0.00%	0.000%
10	3.606	795	798	801	rBV2	387	266	0.02%	0.002%
11	3.664	813	816	821	rVB3	592	467	0.03%	0.004%
12	3.683	821	822	824	rVB	114	23	0.00%	0.000%
13	3.703	824	828	829	rBV2	380	267	0.02%	0.002%
14	3.754	842	844	846	rVB	299	127	0.01%	0.001%
15	3.767	846	848	850	rBV	194	119	0.01%	0.001%
16	3.793	854	856	857	rBV	197	77	0.00%	0.001%
17	3.805	858	860	862	rBV2	294	141	0.01%	0.001%
18	3.860	874	877	880	rBV	420	328	0.02%	0.003%
19	3.950	887	905	924	rBV2	27284	136076	8.56%	1.064%
20	4.342	1015	1027	1055	rVB	244537	619573	38.97%	4.843%
21	5.040	1228	1244	1274	rBV2	639930	1589977	100.00%	12.427%
22	5.612	1410	1422	1448	rBV	486601	1004974	63.21%	7.855%
23	5.902	1501	1512	1518	rBV	40064	81304	5.11%	0.635%
24	6.069	1552	1564	1587	rBV	326475	667376	41.97%	5.216%
25	6.561	1713	1717	1718	rBV2	424	202	0.01%	0.002%
26	6.574	1718	1721	1722	rVV2	317	128	0.01%	0.001%
27	6.616	1730	1734	1737	rBV	486	233	0.01%	0.002%
28	6.645	1737	1743	1751	rVV4	781	758	0.05%	0.006%
29	6.693	1755	1758	1760	rVB2	276	166	0.01%	0.001%
30	6.738	1770	1772	1775	rBV2	266	88	0.01%	0.001%
31	6.825	1797	1799	1800	rVB2	306	96	0.01%	0.001%
32	6.854	1805	1808	1810	rBV	259	156	0.01%	0.001%
33	6.886	1816	1818	1822	rVB2	326	143	0.01%	0.001%
34	6.911	1822	1826	1827	rBV	273	210	0.01%	0.002%
35	6.985	1838	1849	1879	rBV	172783	336838	21.19%	2.633%
36	7.317	1939	1952	1966	rBV	728627	1333981	83.90%	10.427%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021121\
 Data File : VW020297.D
 Acq On : 11 Feb 2021 12:09
 Operator : SY/MD
 Sample : M1375-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BJ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

37	7.622	2037	2047	2079	rBV	121551	230653	14.51%	1.803%
38	8.046	2177	2179	2182	rVB2	552	273	0.02%	0.002%
39	8.063	2182	2184	2185	rBV2	413	157	0.01%	0.001%
40	8.098	2185	2195	2217	rBV	252813	628410	39.52%	4.912%
41	8.577	2341	2344	2348	rBV3	749	509	0.03%	0.004%
42	8.651	2366	2367	2369	rBV2	261	117	0.01%	0.001%
43	8.693	2378	2380	2382	rBV2	532	296	0.02%	0.002%
44	8.747	2396	2397	2398	rBV	275	104	0.01%	0.001%
45	8.786	2407	2409	2410	rBV2	238	92	0.01%	0.001%
46	8.805	2411	2415	2417	rBV2	359	287	0.02%	0.002%
47	8.854	2418	2430	2448	rBV	756314	1324275	83.29%	10.351%
48	9.146	2517	2521	2522	rBV3	732	574	0.04%	0.004%
49	9.175	2529	2530	2533	rBV	353	231	0.01%	0.002%
50	9.198	2535	2537	2538	rBV	430	168	0.01%	0.001%
51	9.291	2564	2566	2572	rBV3	460	402	0.03%	0.003%
52	9.410	2601	2603	2605	rBV2	268	97	0.01%	0.001%
53	9.481	2622	2625	2626	rBV2	238	95	0.01%	0.001%
54	9.654	2675	2679	2680	rBV	225	166	0.01%	0.001%
55	9.738	2700	2705	2709	rBV4	1381	1839	0.12%	0.014%
56	9.812	2726	2728	2730	rBV2	257	153	0.01%	0.001%
57	9.879	2746	2749	2752	rBV2	348	219	0.01%	0.002%
58	9.908	2755	2758	2759	rVV2	210	111	0.01%	0.001%
59	9.960	2770	2774	2775	rBV2	456	272	0.02%	0.002%
60	10.130	2824	2827	2828	rBV3	213	146	0.01%	0.001%
61	10.223	2839	2856	2884	rBV	417734	810124	50.95%	6.332%
62	10.516	2945	2947	2949	rBV2	345	195	0.01%	0.002%
63	10.545	2953	2956	2962	rVV	605	446	0.03%	0.003%
64	10.638	2982	2985	2988	rBV3	361	288	0.02%	0.002%
65	10.825	3041	3043	3045	rBV	367	191	0.01%	0.001%
66	11.040	3108	3110	3114	rVB3	417	232	0.01%	0.002%
67	11.127	3134	3137	3143	rVB2	567	435	0.03%	0.003%
68	11.255	3165	3177	3202	rBV	857459	1421753	89.42%	11.113%
69	11.632	3281	3294	3316	rBV	884067	1468986	92.39%	11.482%
70	11.966	3396	3398	3400	rBV3	469	233	0.01%	0.002%
71	12.056	3423	3426	3430	rBV2	601	457	0.03%	0.004%
72	12.117	3443	3445	3448	rBV2	295	122	0.01%	0.001%
73	12.316	3505	3507	3509	rBV	351	149	0.01%	0.001%
74	12.657	3607	3613	3616	rBV3	987	1047	0.07%	0.008%
75	12.963	3706	3708	3709	rBV	356	138	0.01%	0.001%
76	13.278	3801	3806	3812	rVB6	1726	2014	0.13%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021121\
Data File : VV020297.D
Acq On : 11 Feb 2021 12:09
Operator : SY/MD
Sample : M1375-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BJ5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Title : VOC Analysis

77	13.612	3908	3910	3911	rBV6	369	122	0.01%	0.001%
78	13.760	3950	3956	3961	rBV4	1777	1991	0.13%	0.016%
79	15.271	4419	4426	4434	rBV6	6809	9660	0.61%	0.076%




Sum of corrected areas: 12794049

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021121\
Data File : VV020297.D
Acq On : 11 Feb 2021 12:09
Operator : SY/MD
Sample : M1375-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BJ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

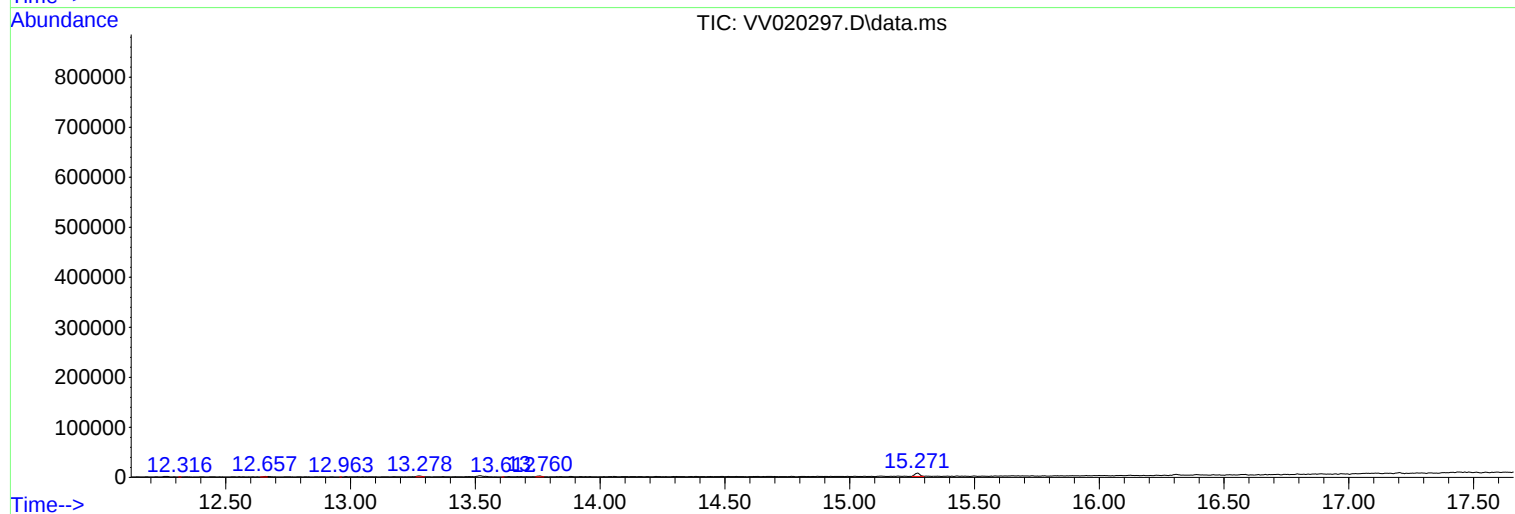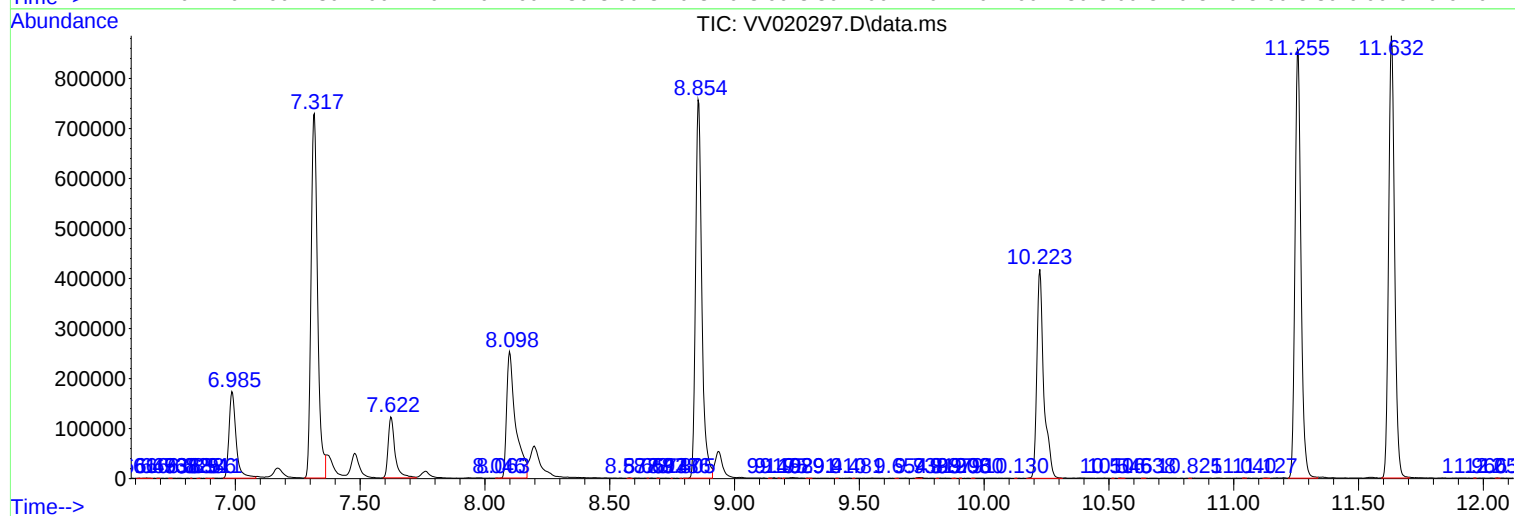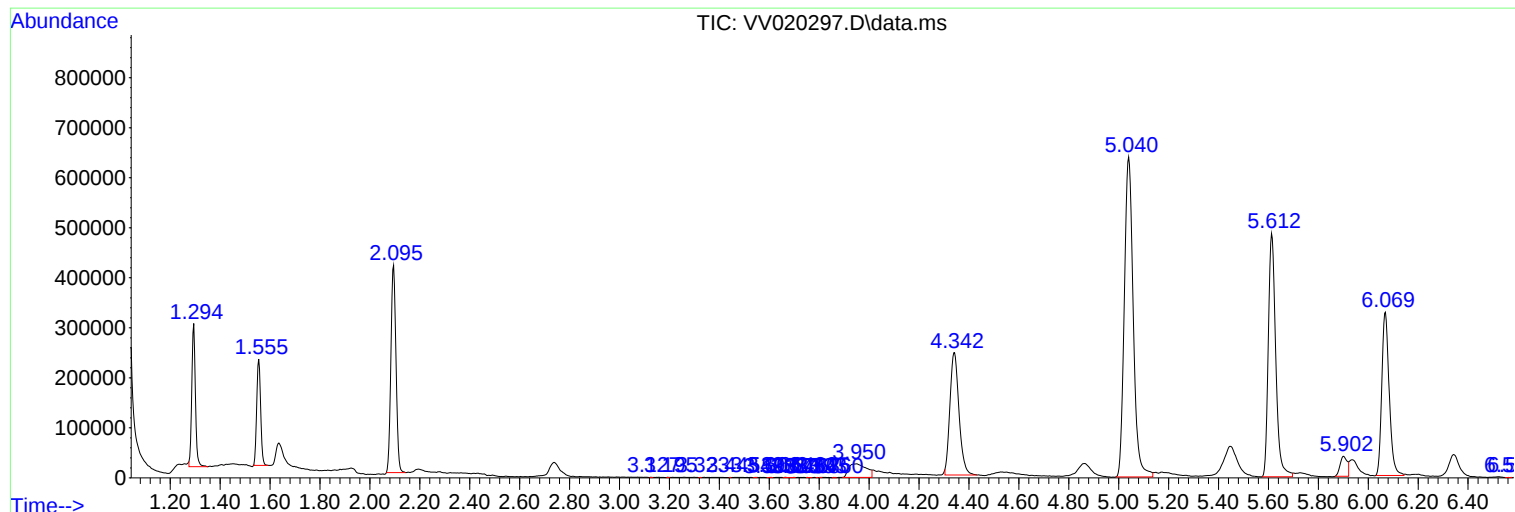

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021121\
Data File : VV020297.D
Acq On : 11 Feb 2021 12:09
Operator : SY/MD
Sample : M1375-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BJ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021121\
Data File : VV020297.D
Acq On : 11 Feb 2021 12:09
Operator : SY/MD
Sample : M1375-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BJ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
