

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021121\
 Data File : VV020305.D
 Acq On : 11 Feb 2021 18:03
 Operator : SY/MD
 Sample : VIBLK03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK03

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

Signal : TIC: VV020305.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	98	rVB	280126	274650	14.17%	1.774%
2	1.568	157	164	180	rVB	233794	264024	13.62%	1.705%
3	2.108	323	332	376	rVB	478597	743937	38.38%	4.805%
4	2.397	420	422	426	rVB4	575	215	0.01%	0.001%
5	2.510	451	457	465	rBV6	2416	3728	0.19%	0.024%
6	2.603	484	486	488	rVB2	506	255	0.01%	0.002%
7	2.629	491	494	497	rBV3	369	277	0.01%	0.002%
8	2.670	505	507	508	rBV	335	125	0.01%	0.001%
9	2.696	513	515	516	rBV	334	141	0.01%	0.001%
10	2.741	527	529	530	rBV	618	241	0.01%	0.002%
11	2.867	566	568	572	rVB3	496	212	0.01%	0.001%
12	2.928	585	587	592	rBV3	265	249	0.01%	0.002%
13	2.950	592	594	597	rVB2	294	173	0.01%	0.001%
14	3.034	617	620	622	rBV2	353	237	0.01%	0.002%
15	3.085	633	636	637	rBV2	338	192	0.01%	0.001%
16	3.121	645	647	649	rBV	266	159	0.01%	0.001%
17	3.159	657	659	661	rVB2	258	98	0.01%	0.001%
18	3.236	680	683	685	rVB2	174	97	0.01%	0.001%
19	3.252	685	688	689	rBV2	297	136	0.01%	0.001%
20	3.262	689	691	699	rVB3	513	511	0.03%	0.003%
21	3.294	699	701	702	rBV	277	100	0.01%	0.001%
22	3.304	702	704	710	rVB3	379	273	0.01%	0.002%
23	3.342	710	716	720	rBV4	377	538	0.03%	0.003%
24	3.378	726	727	728	rBV4	244	67	0.00%	0.000%
25	3.410	735	737	740	rBV2	304	182	0.01%	0.001%
26	3.426	740	742	744	rVV	244	117	0.01%	0.001%
27	3.461	749	753	755	rVV3	415	276	0.01%	0.002%
28	3.490	759	762	763	rVB	372	125	0.01%	0.001%
29	3.500	763	765	766	rBV	186	84	0.00%	0.001%
30	3.506	766	767	771	rVB	357	126	0.01%	0.001%
31	3.523	771	772	773	rBV	183	50	0.00%	0.000%
32	3.532	773	775	777	rVV	208	96	0.00%	0.001%
33	3.545	777	779	780	rVV	227	68	0.00%	0.000%
34	3.568	784	786	788	rBV2	130	87	0.00%	0.001%
35	3.609	795	799	801	rBV2	190	142	0.01%	0.001%
36	3.622	801	803	807	rVB	300	150	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021121\
 Data File : VV020305.D
 Acq On : 11 Feb 2021 18:03
 Operator : SY/MD
 Sample : VIBLK03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK03

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
 Title : VOC Analysis

37	3.641	807	809	811	rBV	287	168	0.01%	0.001%
38	3.651	811	812	815	rBV2	181	83	0.00%	0.001%
39	3.690	821	824	826	rBV	268	199	0.01%	0.001%
40	3.722	831	834	836	rBV	436	296	0.02%	0.002%
41	3.764	842	847	852	rBV2	506	403	0.02%	0.003%
42	3.789	852	855	858	rVB2	475	278	0.01%	0.002%
43	3.895	873	888	926	rBV	125018	409836	21.15%	2.647%
44	4.352	1015	1030	1066	rVB	307683	782615	40.38%	5.055%
45	4.587	1101	1103	1106	rBV2	354	233	0.01%	0.002%
46	4.731	1145	1148	1150	rBV2	258	184	0.01%	0.001%
47	4.783	1162	1164	1168	rBV3	561	472	0.02%	0.003%
48	4.821	1172	1176	1177	rBV2	578	356	0.02%	0.002%
49	4.931	1207	1210	1211	rBV	266	129	0.01%	0.001%
50	4.947	1213	1215	1218	rVB	398	200	0.01%	0.001%
51	4.979	1221	1225	1226	rBV	249	194	0.01%	0.001%
52	5.050	1229	1247	1273	rBV2	760567	1938116	100.00%	12.518%
53	5.358	1341	1343	1349	rVB4	524	368	0.02%	0.002%
54	5.535	1396	1398	1401	rBV	323	199	0.01%	0.001%
55	5.555	1401	1404	1405	rBV	284	150	0.01%	0.001%
56	5.619	1412	1424	1449	rBV	653871	1303575	67.26%	8.419%
57	6.072	1553	1565	1596	rVB	429071	871815	44.98%	5.631%
58	6.413	1669	1671	1678	rBV5	712	694	0.04%	0.004%
59	6.940	1833	1835	1837	rBV2	226	133	0.01%	0.001%
60	6.989	1839	1850	1875	rVV	230853	418634	21.60%	2.704%
61	7.320	1941	1953	1976	rBV	895162	1544681	79.70%	9.977%
62	7.625	2038	2048	2067	rBV	160343	277900	14.34%	1.795%
63	7.879	2125	2127	2130	rBV2	352	230	0.01%	0.001%
64	8.005	2164	2166	2171	rVB5	480	343	0.02%	0.002%
65	8.024	2171	2172	2173	rVB	332	64	0.00%	0.000%
66	8.037	2173	2176	2177	rBV2	344	177	0.01%	0.001%
67	8.091	2183	2193	2230	rBV	489671	907313	46.81%	5.860%
68	8.484	2312	2315	2319	rVB4	769	591	0.03%	0.004%
69	8.644	2362	2365	2370	rBV4	767	583	0.03%	0.004%
70	8.680	2375	2376	2380	rVB2	528	330	0.02%	0.002%
71	8.706	2381	2384	2385	rBV2	640	304	0.02%	0.002%
72	8.735	2391	2393	2395	rBV	359	210	0.01%	0.001%
73	8.857	2419	2431	2459	rBV	994762	1625207	83.85%	10.497%
74	9.146	2518	2521	2523	rBV3	368	197	0.01%	0.001%
75	9.207	2536	2540	2543	rBV3	302	248	0.01%	0.002%
76	9.223	2543	2545	2551	rBV2	647	510	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021121\
 Data File : VW020305.D
 Acq On : 11 Feb 2021 18:03
 Operator : SY/MD
 Sample : VIBLK03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK03

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

77	9.352	2583	2585	2586	rBV	209	97	0.01%	0.001%
78	9.387	2593	2596	2599	rBV	343	241	0.01%	0.002%
79	9.535	2640	2642	2646	rVB3	474	296	0.02%	0.002%
80	9.551	2646	2647	2648	rBV3	193	42	0.00%	0.000%
81	9.587	2655	2658	2661	rBV	364	235	0.01%	0.002%
82	9.667	2681	2683	2686	rVB2	638	314	0.02%	0.002%
83	9.789	2714	2721	2723	rBV3	456	562	0.03%	0.004%
84	9.908	2755	2758	2760	rBV2	471	324	0.02%	0.002%
85	9.979	2776	2780	2782	rBV2	488	318	0.02%	0.002%
86	10.223	2842	2856	2884	rBV	612012	969468	50.02%	6.261%
87	10.410	2912	2914	2918	rVB3	546	304	0.02%	0.002%
88	10.471	2931	2933	2937	rBV	373	329	0.02%	0.002%
89	10.567	2960	2963	2965	rBV2	311	191	0.01%	0.001%
90	10.580	2965	2967	2973	rVB4	585	452	0.02%	0.003%
91	10.609	2973	2976	2978	rBV2	248	150	0.01%	0.001%
92	10.728	3010	3013	3016	rVB	423	255	0.01%	0.002%
93	10.879	3058	3060	3063	rVB2	489	176	0.01%	0.001%
94	10.892	3063	3064	3067	rBV	354	170	0.01%	0.001%
95	11.255	3165	3177	3200	rBV	1042017	1601727	82.64%	10.345%
96	11.632	3280	3294	3313	rBV	976897	1526519	78.76%	9.859%
97	12.696	3623	3625	3629	rBV2	583	429	0.02%	0.003%
98	13.355	3827	3830	3831	rBV	439	229	0.01%	0.001%




Sum of corrected areas: 15483184

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021121\
Data File : VV020305.D
Acq On : 11 Feb 2021 18:03
Operator : SY/MD
Sample : VIBLK03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

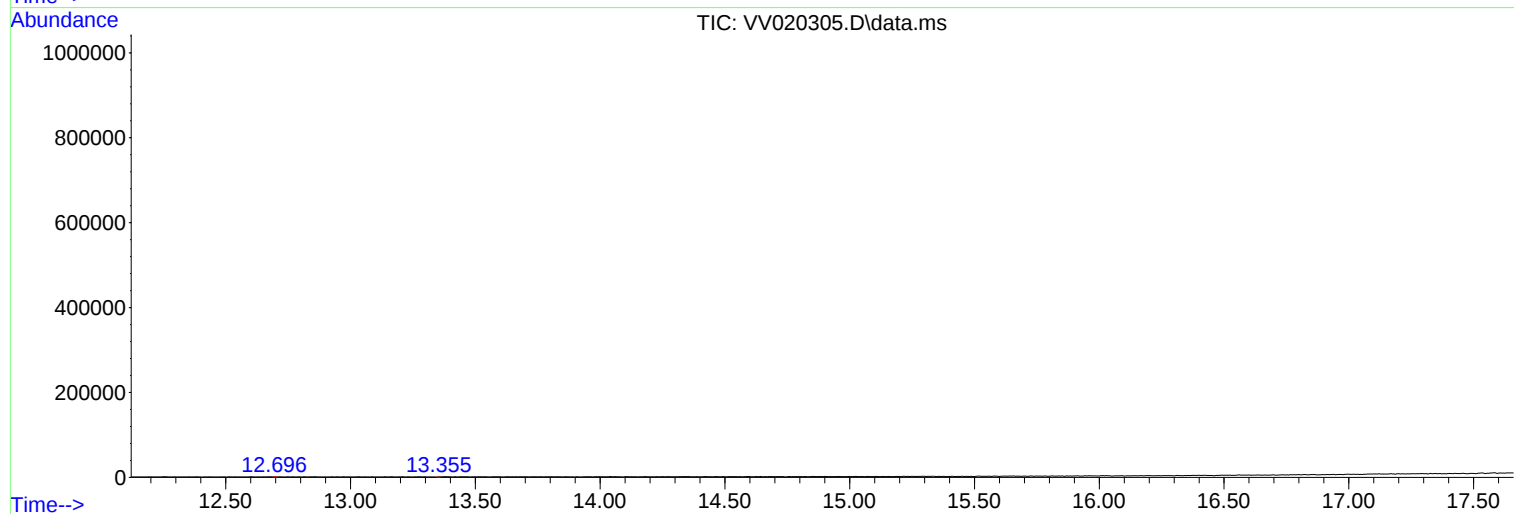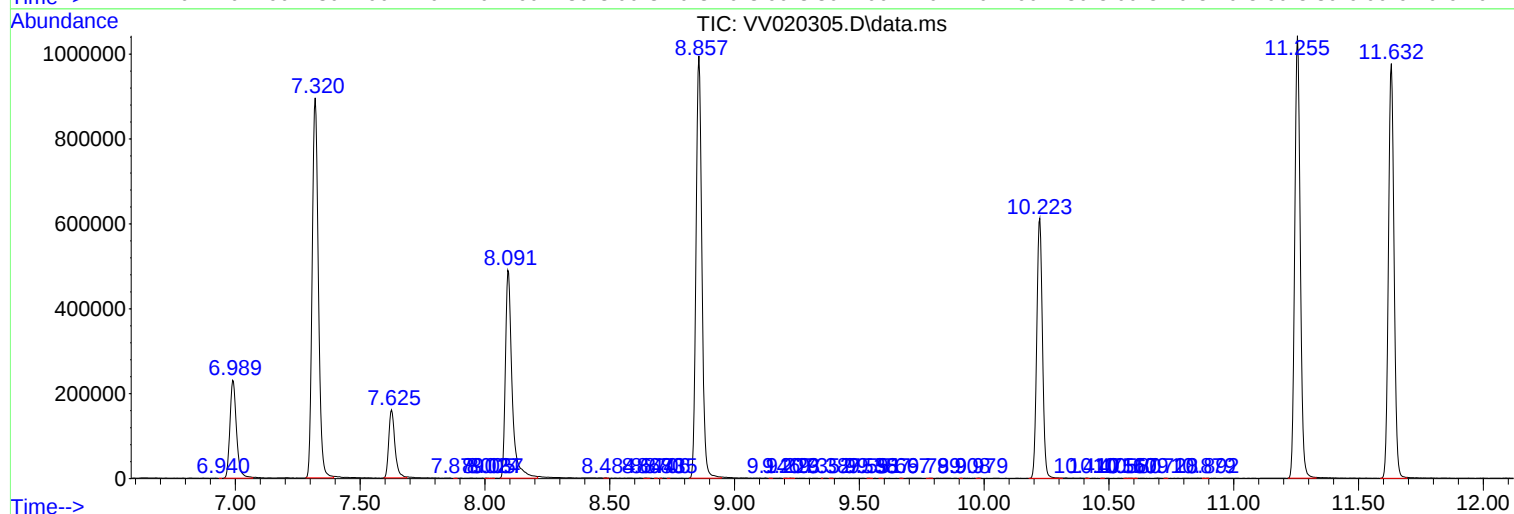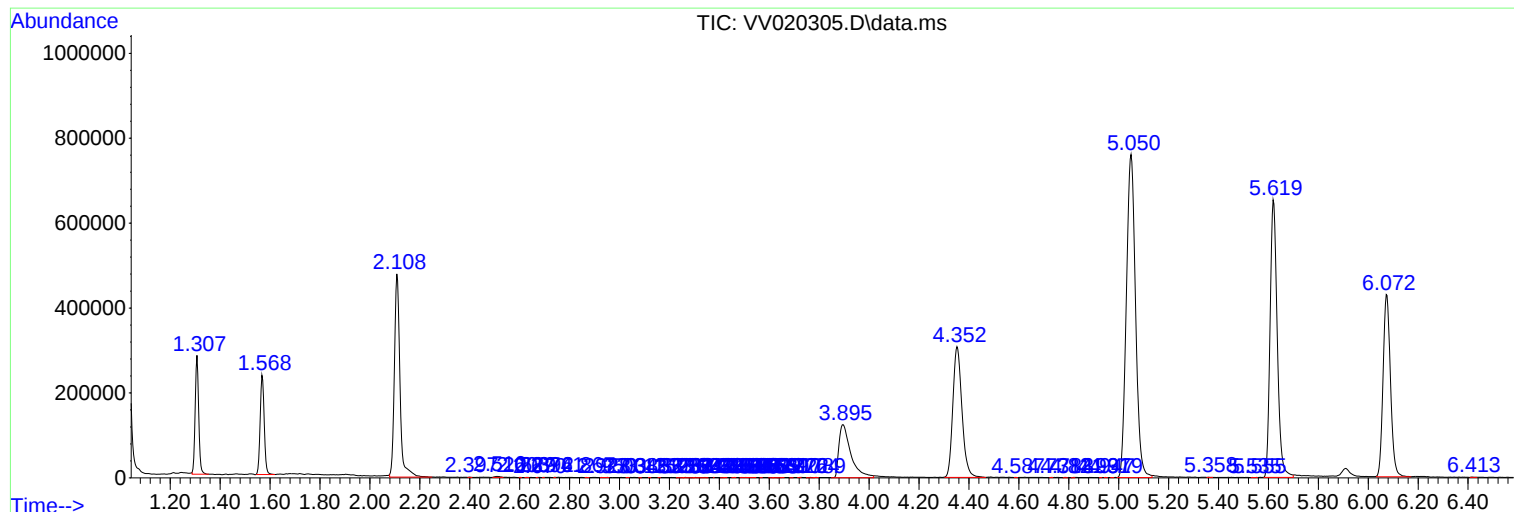

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021121\
Data File : VV020305.D
Acq On : 11 Feb 2021 18:03
Operator : SY/MD
Sample : VIBLK03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021121\
Data File : VV020305.D
Acq On : 11 Feb 2021 18:03
Operator : SY/MD
Sample : VIBLK03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
