


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021121\
 Data File : VV020292.D
 Acq On : 11 Feb 2021 08:43
 Operator : SY/MD
 Sample : BFB89
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB89

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
 Title : VOC Analysis
 Last Update : Fri Feb 12 00:25:49 2021

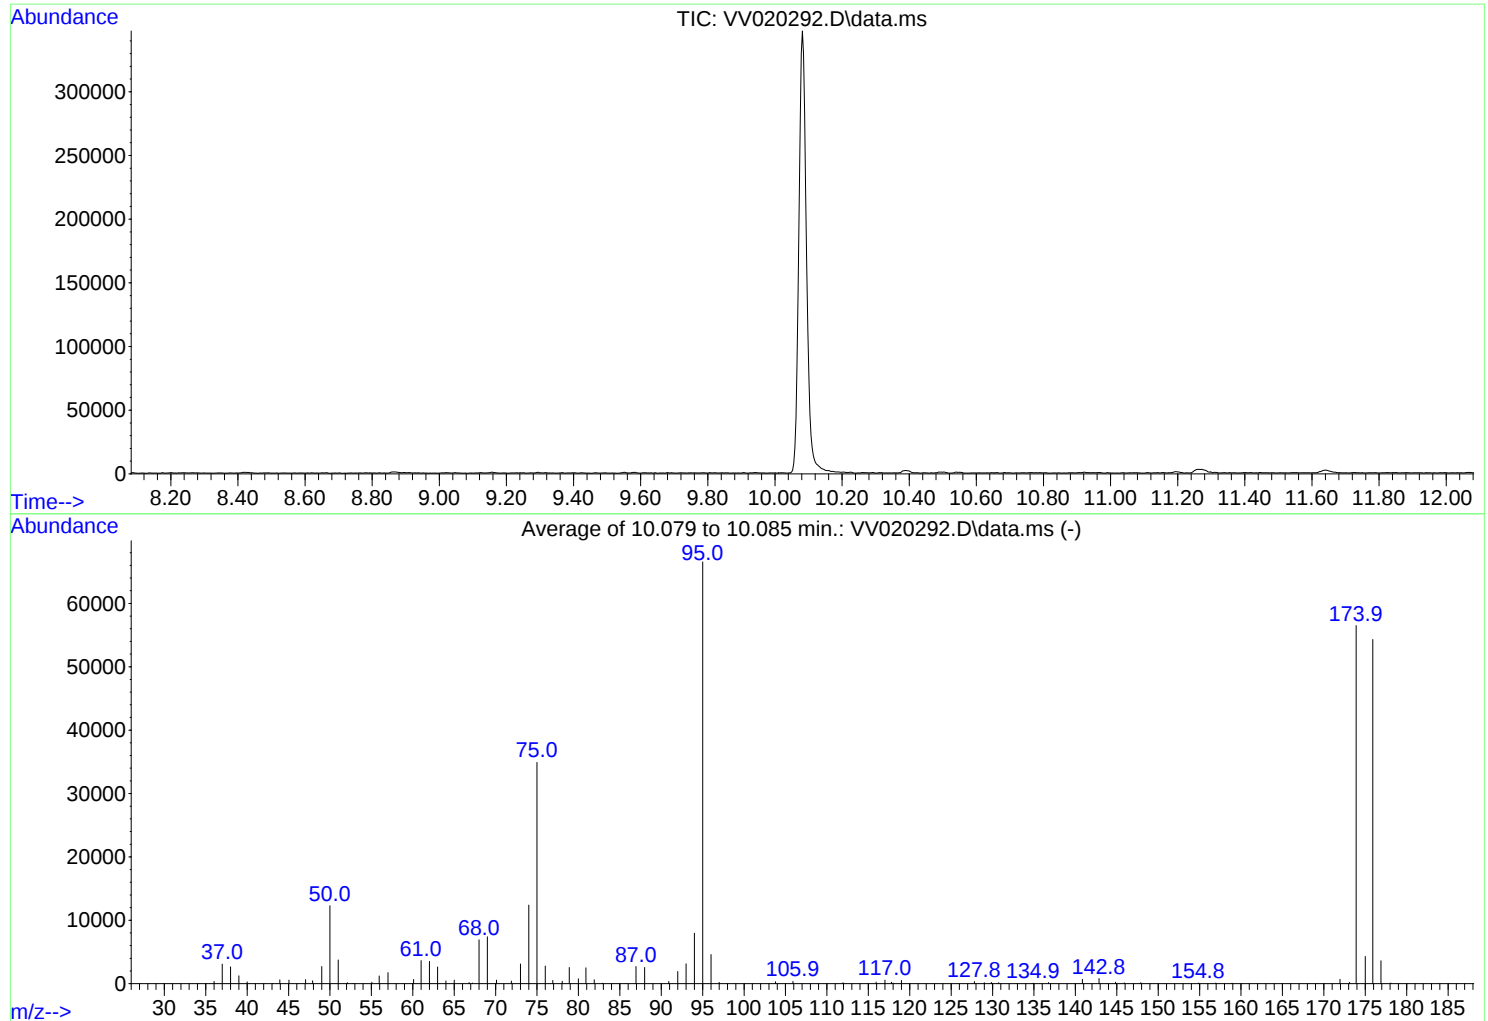

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2800

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	12307	PASS
75	95	30	80	52.5	34925	PASS
95	95	100	100	100.0	66557	PASS
96	95	5	9	6.9	4603	PASS
173	174	0.00	2	0.4	201	PASS
174	95	50	120	84.9	56512	PASS
175	174	5	9	7.6	4300	PASS
176	174	95	101	96.1	54301	PASS
177	176	5	9	6.6	3605	PASS

m/z	Abundance
36.00	488.0
37.00	3024.0
38.00	2656.0
39.00	1287.0
40.00	286.0
44.00	1018.0
45.10	545.0
47.00	569.0
47.90	425.0
49.00	2834.0
50.00	12355.0
51.00	3807.0
55.00	204.0
56.00	1203.0
57.00	1853.0
60.10	615.0
61.00	3788.0
62.00	3562.0
63.00	2674.0
64.00	451.0
65.00	479.0
66.80	177.0
67.20	172.0
68.00	6761.0
69.00	7358.0
70.10	563.0
71.90	403.0
73.00	3344.0
74.00	12165.0
75.00	35112.0
76.00	2668.0
76.90	435.0
78.10	416.0
78.90	2520.0
80.00	769.0
80.90	2325.0
81.90	567.0
86.90	2766.0
88.00	2638.0
90.90	380.0
92.00	1955.0
93.00	3108.0
94.00	7903.0
95.00	65864.0
96.00	4642.0
97.00	167.0
103.80	303.0
105.90	363.0
111.90	166.0
116.00	244.0
117.00	548.0
117.80	221.0
118.00	227.0
119.00	470.0
127.80	350.0
129.00	148.0
129.80	205.0
130.70	152.0
136.70	116.0
140.80	691.0
142.90	883.0
144.80	195.0
145.90	119.0
147.80	179.0
154.80	115.0
157.00	103.0
172.00	722.0
173.90	54096.0
175.00	4231.0
175.90	52032.0
176.90	3557.0
178.10	173.0

Instrument :
MSVOA_V
ClientSampleId :
BFB89

m/z	Abundance
36.00	506.0
37.00	3187.0
38.00	2736.0
39.00	1269.0
40.00	281.0
44.00	1104.0
45.00	576.0
47.10	656.0
47.90	479.0
49.00	2753.0
50.00	12630.0
51.00	3873.0
52.10	198.0
55.10	229.0
55.90	1301.0
57.00	1771.0
60.10	683.0
61.00	3796.0
62.00	3583.0
63.00	2657.0
64.00	448.0
65.00	581.0
66.80	184.0
67.20	157.0
68.00	7163.0
69.00	7723.0
70.10	576.0
71.90	419.0
73.00	3145.0
74.00	12918.0
75.00	36168.0
76.00	2892.0
76.90	539.0
78.10	414.0
78.90	2652.0
80.00	790.0
80.90	2584.0
81.90	626.0
82.90	118.0
85.70	103.0
87.00	2814.0
88.00	2611.0
90.90	375.0
92.00	2007.0
93.00	3254.0
94.00	8176.0
95.00	68992.0
96.00	4831.0
97.00	219.0
103.80	308.0
105.90	384.0
112.00	173.0
115.90	263.0
117.00	578.0
117.80	234.0
119.00	548.0
127.80	327.0
129.00	154.0
129.90	218.0
130.80	153.0
134.90	102.0
136.80	191.0
140.80	698.0
142.80	849.0
144.90	228.0
145.90	154.0
147.90	159.0
154.80	110.0
157.00	108.0
158.90	117.0
172.00	692.0
173.90	58520.0
175.00	4521.0
175.90	56344.0
176.90	3730.0
178.10	127.0

Instrument :
MSVOA_V
ClientSampleId :
BFB89

m/z	Abundance
36.00	459.0
37.00	3069.0
38.00	2572.0
39.00	1146.0
40.00	278.0
43.10	106.0
44.00	1062.0
45.00	565.0
47.10	682.0
47.90	483.0
49.00	2511.0
50.00	11936.0
51.00	3571.0
52.10	226.0
52.80	117.0
55.10	251.0
55.90	1145.0
57.00	1624.0
60.10	692.0
61.00	3345.0
62.00	3388.0
63.00	2524.0
64.00	399.0
65.00	617.0
66.80	211.0
68.00	6856.0
69.00	7102.0
70.10	550.0
71.90	403.0
73.00	2816.0
74.00	12117.0
75.00	33496.0
76.00	2783.0
76.90	583.0
78.00	336.0
78.90	2475.0
80.00	727.0
80.90	2623.0
81.90	596.0
82.90	111.0
87.00	2560.0
88.00	2437.0
90.90	331.0
92.00	1794.0
93.00	3052.0
94.00	7788.0
95.00	64816.0
96.00	4336.0
97.00	191.0
103.80	268.0
105.90	353.0
112.00	132.0
115.90	252.0
117.00	520.0
117.80	220.0
119.00	531.0
127.80	313.0
129.00	138.0
129.90	218.0
130.80	137.0
134.90	108.0
136.80	215.0
140.90	642.0
142.90	716.0
144.90	240.0
145.90	122.0
148.00	133.0
154.90	110.0
156.90	103.0
158.90	135.0
171.90	627.0
173.10	603.0
173.90	56920.0
175.00	4148.0
175.90	54528.0
176.90	3528.0

Instrument :
MSVOA_V
ClientSampleId :
BFB89

m/z	Abundance
36.10	118.0
39.70	173.0
43.90	454.0

Instrument :
MSVOA_V
ClientSampleId :
BFB89