


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV021219\
 Data File : VV009281.D
 Acq On : 12 Feb 2019 11:43
 Operator : SY/MD
 Sample : BFB61
 Misc : 5.00G/10ML/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB61

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM021219S.M
 Title : VOC Analysis
 Last Update : Wed Feb 13 07:40:48 2019

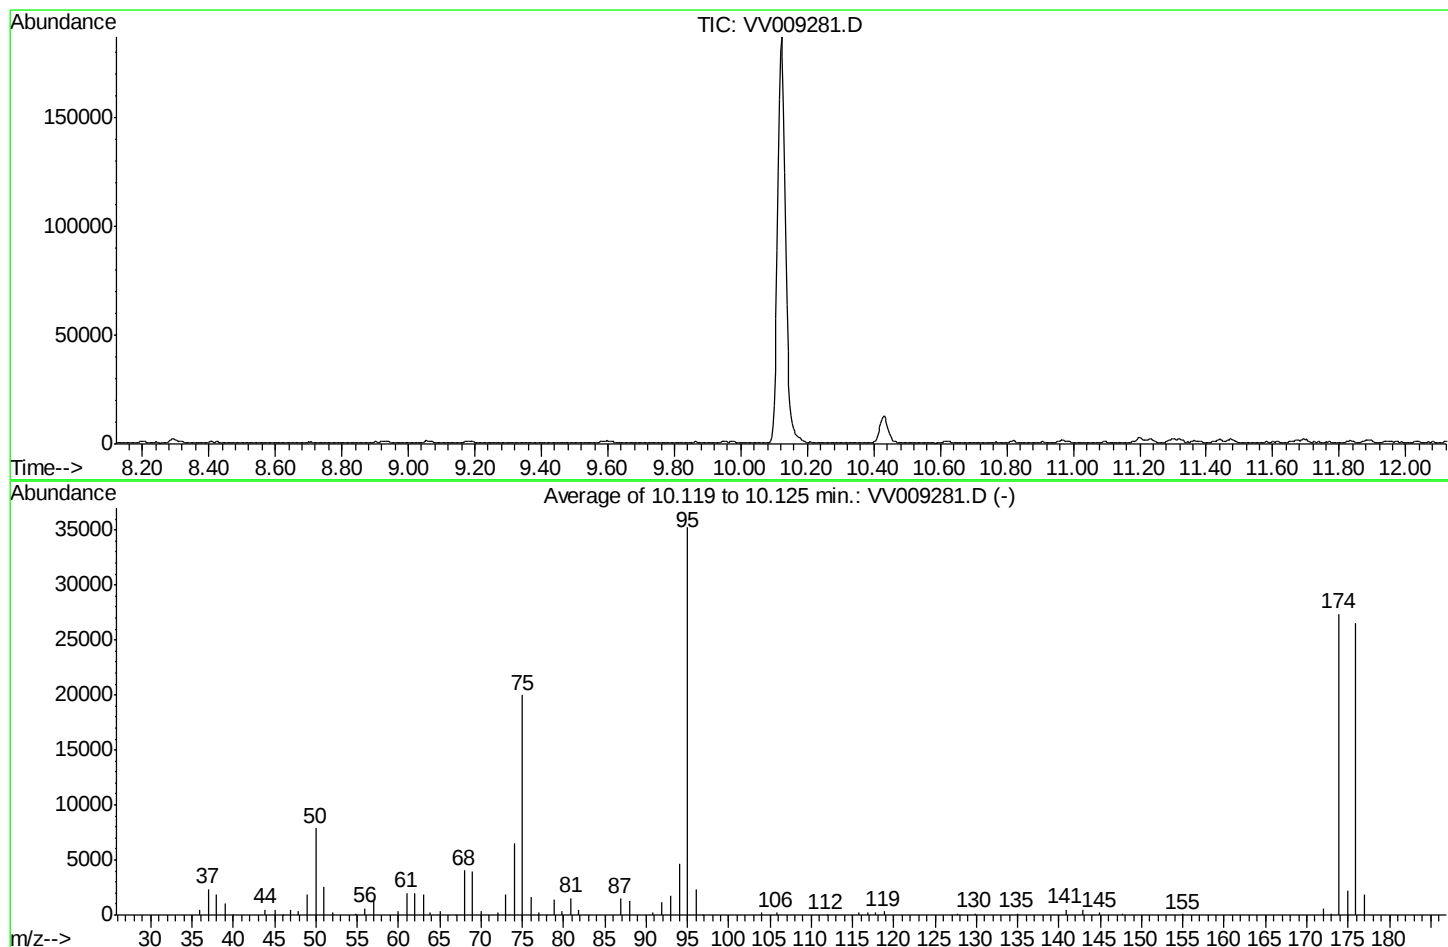

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	7877	PASS
75	95	30	80	56.6	19957	PASS
95	95	100	100	100.0	35234	PASS
96	95	5	9	6.6	2310	PASS
173	174	0.00	2	0.4	111	PASS
174	95	50	120	77.6	27352	PASS
175	174	5	9	7.9	2156	PASS
176	174	95	101	97.2	26578	PASS
177	176	5	9	7.1	1884	PASS

m/z	Abundance
35.90	440.0
37.00	2393.0
38.00	2034.0
39.00	1036.0
39.80	194.0
44.00	760.0
45.00	350.0
46.00	104.0
47.00	446.0
47.90	317.0
49.00	1704.0
50.00	7962.0
51.00	2546.0
52.00	169.0
55.00	157.0
56.00	593.0
57.00	1315.0
59.90	334.0
61.00	1996.0
62.00	1955.0
63.00	1971.0
63.80	263.0
65.00	407.0
68.00	3849.0
69.00	3937.0
70.00	323.0
72.00	219.0
73.00	1768.0
74.00	6393.0
75.00	20320.0
76.00	1589.0
77.00	212.0
78.90	1437.0
79.80	345.0
80.90	1623.0
81.80	460.0
86.90	1509.0
87.90	1337.0
90.90	237.0
91.90	1205.0
92.90	1670.0
94.00	4626.0
95.00	35360.0
96.00	2381.0
103.90	169.0
105.80	178.0
115.70	201.0
116.80	287.0
117.90	227.0
118.80	380.0
127.70	154.0
129.80	170.0
134.90	128.0
140.80	484.0
142.90	458.0
145.00	201.0
147.70	128.0
155.00	139.0
171.90	576.0
173.90	26816.0
175.00	2168.0
175.90	25672.0
176.90	1888.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61

m/z	Abundance
35.90	436.0
37.00	2455.0
38.00	1931.0
39.00	1018.0
39.90	199.0
44.00	821.0
45.00	477.0
47.00	482.0
47.90	360.0
49.00	1928.0
50.00	8115.0
51.00	2636.0
52.00	196.0
54.90	176.0
56.00	598.0
57.00	1296.0
59.90	335.0
61.00	2037.0
62.00	1969.0
63.00	1863.0
63.80	220.0
65.00	409.0
68.00	4164.0
69.00	4097.0
69.90	333.0
72.00	280.0
73.00	1907.0
74.00	6761.0
75.00	20544.0
76.00	1600.0
77.00	206.0
78.90	1467.0
79.90	350.0
80.90	1577.0
81.90	445.0
86.90	1519.0
88.00	1387.0
90.90	203.0
91.90	1168.0
92.90	1829.0
94.00	4885.0
95.00	36360.0
96.00	2340.0
103.90	184.0
105.80	227.0
115.80	190.0
116.80	290.0
117.80	199.0
118.90	315.0
127.70	130.0
129.80	153.0
134.90	136.0
140.80	527.0
142.90	493.0
144.90	221.0
147.70	140.0
155.00	110.0
172.00	598.0
173.90	28128.0
175.00	2261.0
175.90	27472.0
176.90	1890.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61

m/z	Abundance
35.90	425.0
37.00	2280.0
38.00	1761.0
39.00	987.0
39.90	234.0
43.90	764.0
45.00	554.0
47.00	468.0
47.90	336.0
49.00	1827.0
50.00	7554.0
51.00	2484.0
52.10	195.0
54.80	181.0
55.90	571.0
57.00	1116.0
59.90	391.0
61.00	1957.0
62.00	1851.0
63.00	1729.0
63.90	173.0
65.00	387.0
66.90	134.0
68.00	4079.0
69.00	3931.0
69.90	326.0
72.00	303.0
73.00	1863.0
74.00	6552.0
75.00	19008.0
76.00	1547.0
77.00	215.0
78.00	107.0
78.90	1391.0
79.90	406.0
80.90	1412.0
81.90	432.0
86.90	1502.0
88.00	1271.0
90.80	150.0
92.00	1030.0
92.90	1782.0
94.00	4616.0
95.00	33984.0
96.00	2210.0
96.90	103.0
103.90	190.0
105.80	227.0
111.80	117.0
115.80	172.0
116.80	259.0
117.70	210.0
118.80	204.0
127.80	126.0
129.80	139.0
134.90	119.0
140.80	523.0
142.90	510.0
144.90	210.0
147.80	147.0
171.90	527.0
173.00	335.0
173.90	27112.0
174.90	2040.0
175.90	26592.0
176.90	1874.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61

m/z	Abundance
40.00	182.0
43.90	292.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61