


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV021220\
 Data File : VV014562.D
 Acq On : 12 Feb 2020 08:57
 Operator : SY/MD
 Sample : BFB89
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB89

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
 Title : VOC Analysis
 Last Update : Thu Feb 13 05:55:11 2020

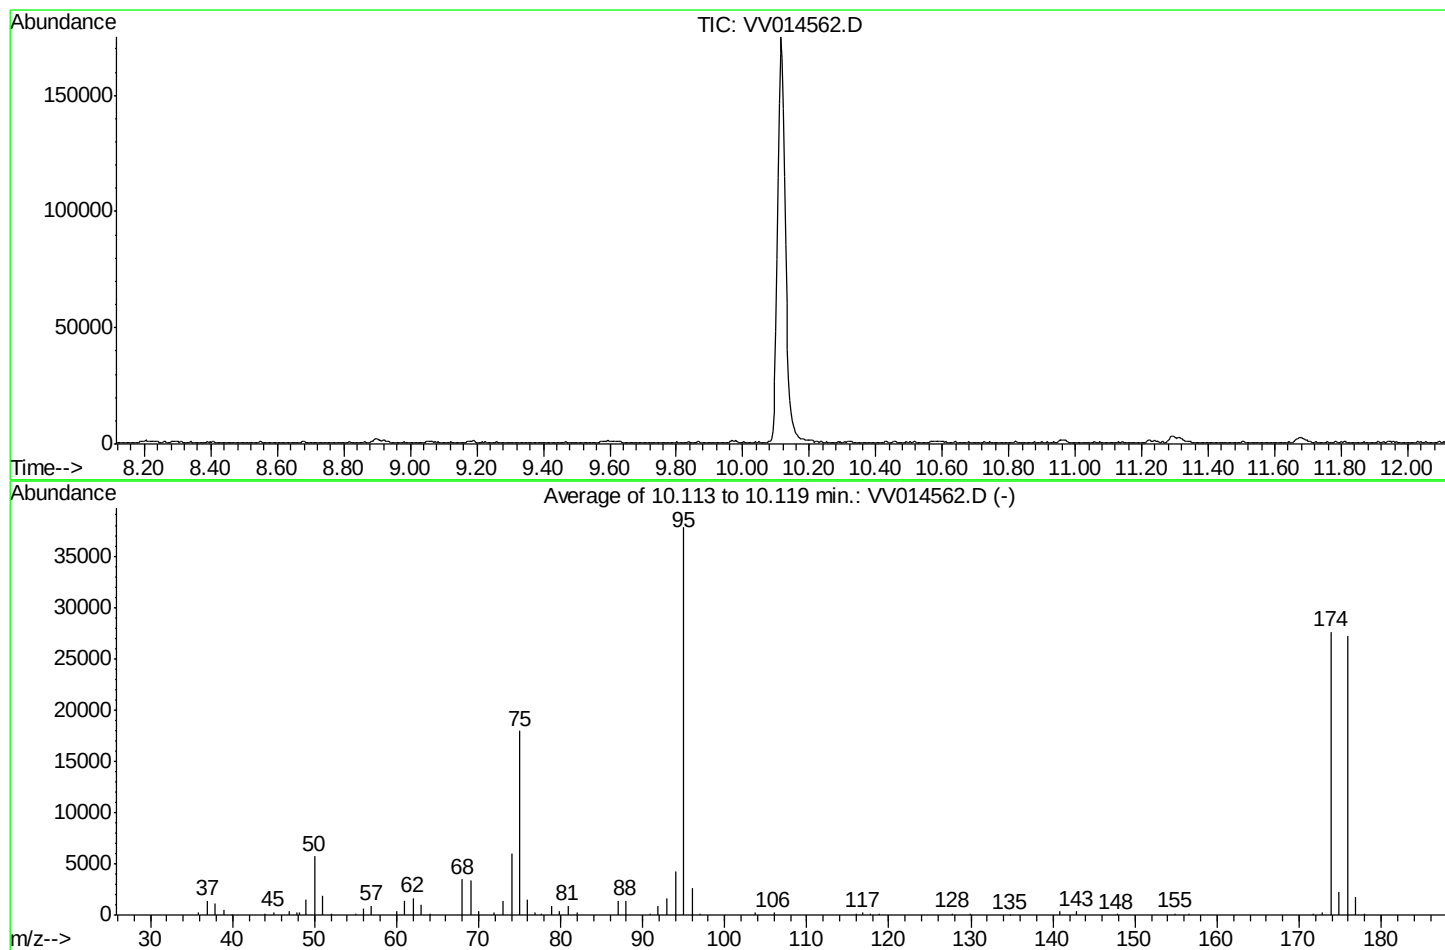

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.1	5710	PASS
75	95	30	80	47.5	17944	PASS
95	95	100	100	100.0	37792	PASS
96	95	5	9	6.8	2569	PASS
173	174	0.00	2	0.9	256	PASS
174	95	50	120	73.1	27610	PASS
175	174	5	9	8.0	2202	PASS
176	174	95	101	98.5	27189	PASS
177	176	5	9	6.4	1748	PASS

m/z	Abundance
35.90	348.0
37.00	1460.0
37.90	1315.0
38.90	526.0
40.00	257.0
43.00	129.0
43.90	476.0
45.00	320.0
46.90	418.0
47.80	228.0
48.10	241.0
49.00	1539.0
50.00	5660.0
51.00	1959.0
52.00	150.0
54.90	108.0
55.90	548.0
56.90	882.0
60.00	400.0
61.00	1481.0
62.00	1670.0
63.00	1076.0
64.00	148.0
68.00	3442.0
69.00	3458.0
70.00	362.0
71.90	262.0
73.00	1391.0
74.00	5789.0
75.00	18024.0
76.00	1566.0
77.00	258.0
78.90	951.0
79.90	312.0
80.90	870.0
82.00	220.0
87.00	1434.0
87.90	1447.0
90.80	156.0
91.90	892.0
93.00	1595.0
94.00	4266.0
95.00	38016.0
96.00	2617.0
103.70	187.0
106.00	217.0
116.00	174.0
116.90	232.0
117.70	161.0
118.90	192.0
127.80	158.0
129.90	119.0
140.80	276.0
142.90	329.0
147.80	118.0
154.90	138.0
156.60	122.0
171.80	126.0
172.80	383.0
173.90	26624.0
174.90	2184.0
175.90	26104.0
176.90	1632.0
178.00	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB89

m/z	Abundance
35.90	321.0
37.00	1431.0
37.90	1286.0
38.90	543.0
39.90	247.0
43.90	465.0
45.00	307.0
46.90	465.0
47.80	238.0
48.10	246.0
49.00	1477.0
50.00	5944.0
51.00	2001.0
52.10	137.0
55.00	117.0
55.90	618.0
57.00	935.0
60.00	365.0
61.00	1492.0
62.00	1692.0
63.00	961.0
64.10	163.0
68.00	3550.0
69.00	3440.0
69.90	347.0
71.90	308.0
73.00	1420.0
74.00	6125.0
75.00	18520.0
76.00	1523.0
76.90	196.0
77.70	147.0
78.90	948.0
79.90	343.0
80.90	929.0
81.90	245.0
87.00	1457.0
87.90	1495.0
90.90	138.0
91.90	927.0
93.00	1663.0
94.00	4388.0
95.00	38976.0
96.00	2655.0
96.90	115.0
103.70	205.0
106.00	208.0
116.00	153.0
116.80	242.0
117.70	204.0
118.80	197.0
127.80	189.0
129.90	128.0
140.80	332.0
142.90	391.0
147.80	115.0
154.90	162.0
156.60	111.0
171.80	126.0
172.80	385.0
173.90	28296.0
174.90	2260.0
175.90	28176.0
176.90	1842.0
177.90	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB89

m/z	Abundance
35.90	279.0
37.00	1393.0
37.90	1104.0
38.90	510.0
39.80	228.0
44.00	486.0
45.00	249.0
47.00	442.0
47.80	242.0
48.10	233.0
48.90	1372.0
50.00	5528.0
51.00	1819.0
52.10	111.0
54.90	124.0
55.90	624.0
57.00	953.0
59.90	278.0
61.00	1337.0
62.00	1548.0
63.00	813.0
64.10	157.0
68.00	3327.0
69.00	3126.0
69.90	364.0
71.90	289.0
73.00	1367.0
74.00	5917.0
75.00	17288.0
76.00	1410.0
76.80	172.0
77.70	157.0
78.90	897.0
79.90	338.0
80.90	986.0
81.90	267.0
87.00	1318.0
87.90	1366.0
91.00	169.0
91.90	938.0
92.90	1575.0
94.00	4037.0
95.00	36384.0
96.00	2436.0
97.00	117.0
103.70	189.0
106.00	184.0
115.90	127.0
116.80	233.0
117.70	171.0
118.80	180.0
127.80	195.0
129.90	122.0
134.80	101.0
140.80	387.0
142.90	385.0
147.90	106.0
154.90	143.0
171.70	107.0
174.00	27912.0
174.90	2162.0
175.90	27288.0
176.80	1771.0
177.90	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB89

Scan 2795 (10.077 min): VV014562.D
BFB89

m/z	Abundance
36.10	101.0
37.70	118.0
39.90	193.0
43.20	104.0
44.00	337.0
51.60	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB89