

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021221\
 Data File : VW020312.D
 Acq On : 12 Feb 2021 12:56
 Operator : SY/MD
 Sample : M1330-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Quant Time: Feb 12 22:15:23 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Feb 12 22:14:10 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	542240	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	527871	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.256	152	259062	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	142270	35.99	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	71.98%		
7) Chloroethane-d5	1.568	69	141633	43.67	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	87.34%		
11) 1,1-Dichloroethene-d2	2.108	63	227272	30.41	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	60.82%		
21) 2-Butanone-d5	3.876	46	219902	99.56	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	99.56%		
24) Chloroform-d	4.349	84	316906	45.05	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.10%		
26) 1,2-Dichloroethane-d4	5.031	65	222742	49.94	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.88%		
32) Benzene-d6	5.050	84	632814	46.27	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.54%		
36) 1,2-Dichloropropane-d6	6.069	67	204592	50.11	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	100.22%		
41) Toluene-d8	7.317	98	566820	44.10	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	88.20%		
43) trans-1,3-Dichloroprop...	7.622	79	89660	43.08	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	86.16%		
47) 2-Hexanone-d5	8.088	63	145492	85.65	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	85.65%		
57) 1,1,2,2-Tetrachloroeth...	10.220	84	277115	47.27	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	94.54%		
64) 1,2-Dichlorobenzene-d4	11.632	152	244105	49.80	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	99.60%		
Target Compounds					Qvalue	
25) Chloroform	4.378	83	9996	1.51	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021221\
Data File : VV020312.D
Acq On : 12 Feb 2021 12:56
Operator : SY/MD
Sample : M1330-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Time: Feb 12 22:15:23 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 12 22:14:10 2021
Response via : Initial Calibration

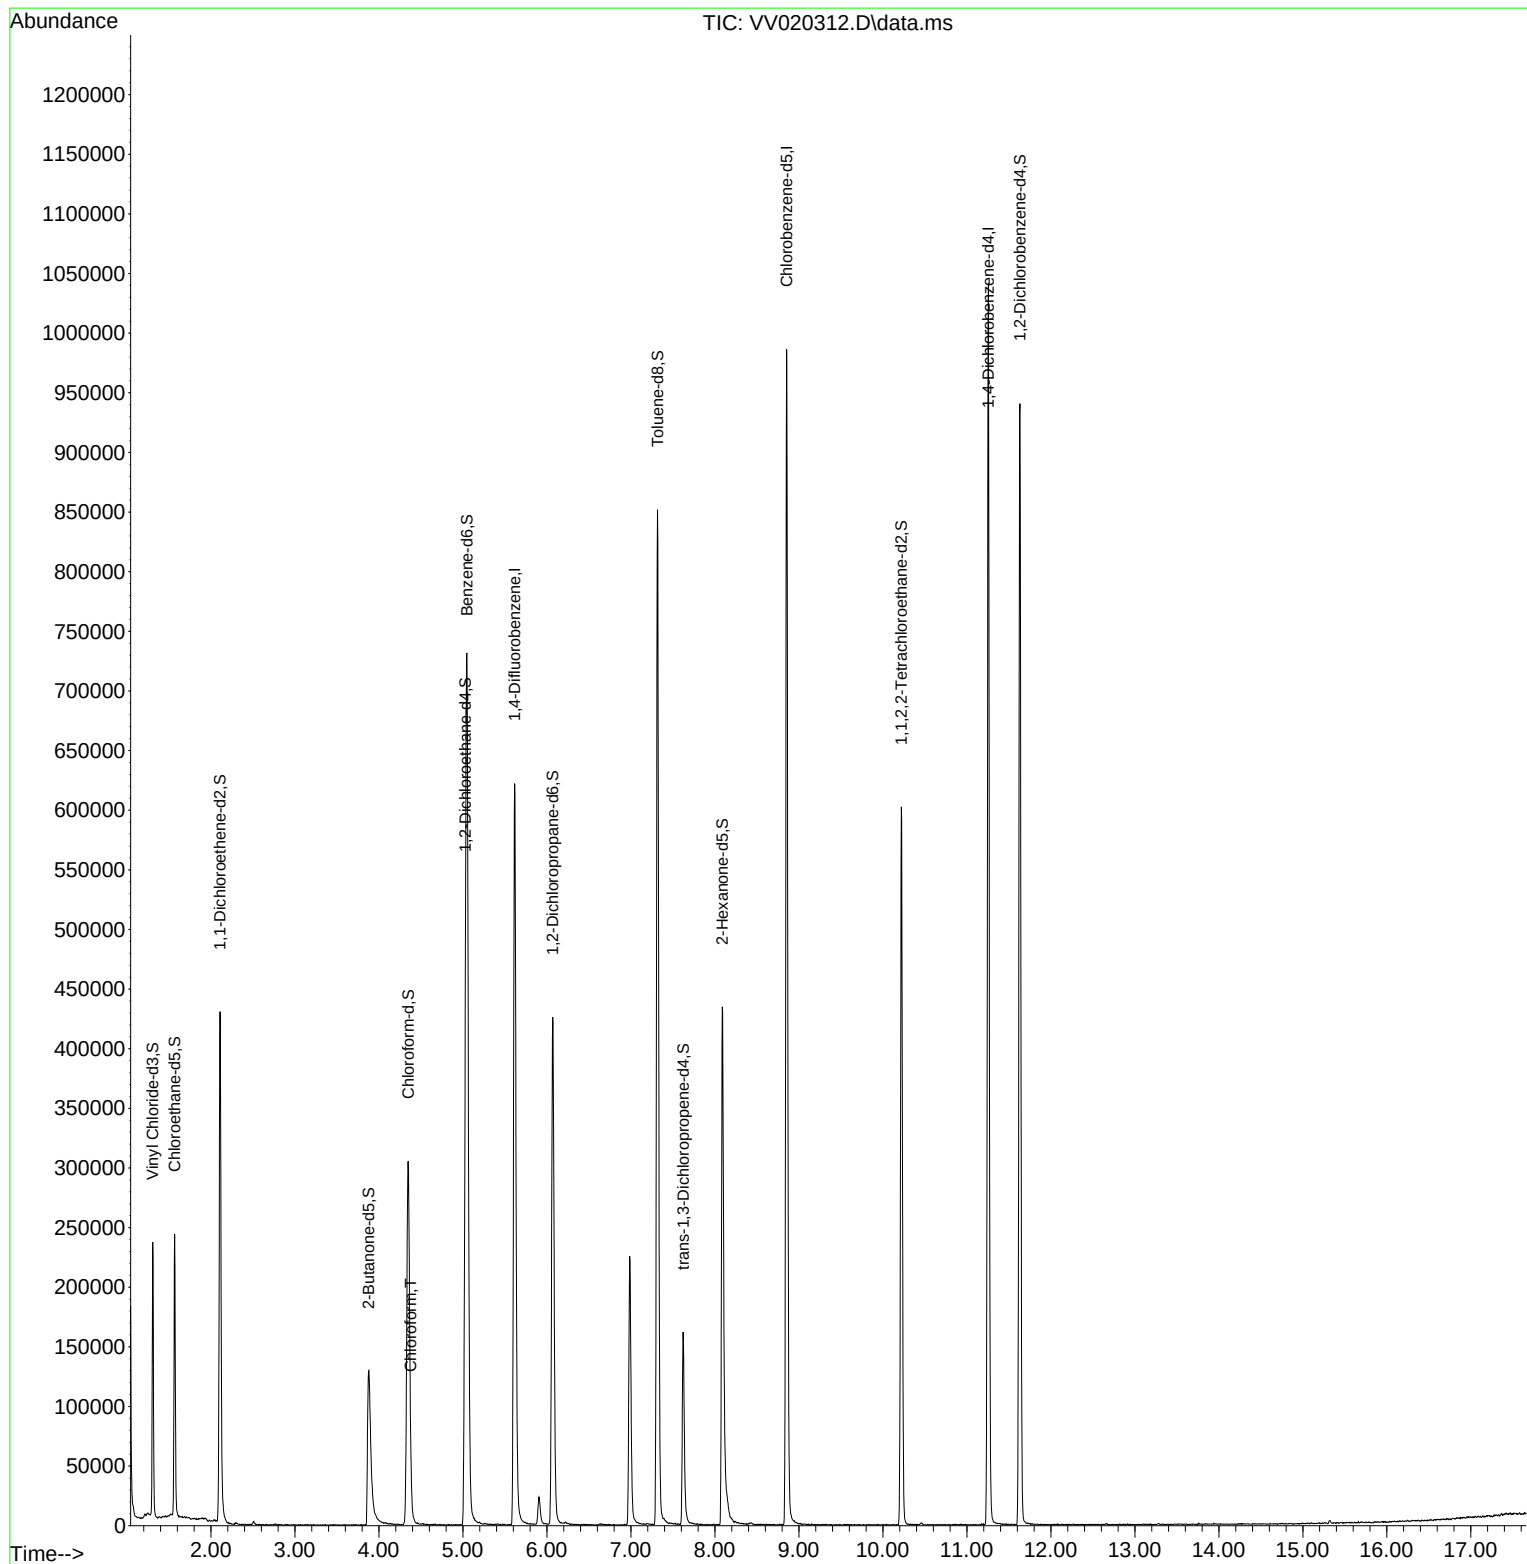

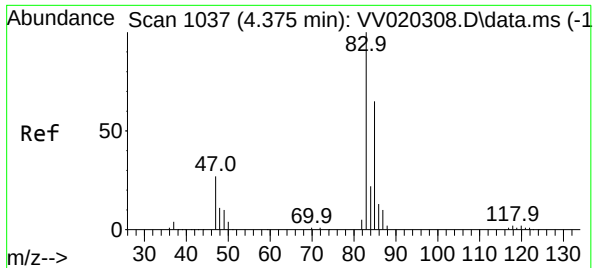

#25
 Chloroform
 Concen: 1.51 ug/L
 RT: 4.378 min Scan# 1038
 Delta R.T. 0.003 min
 Lab File: VV020312.D
 Acq: 12 Feb 2021 12:56

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Tgt Ion: 83 Resp: 9996
 Ion Ratio Lower Upper
 83 100
 85 66.8 44.2 82.2

