

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021221\
 Data File : VW020312.D
 Acq On : 12 Feb 2021 12:56
 Operator : SY/MD
 Sample : M1330-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

Signal : TIC: VW020312.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	100	rVB	230961	236422	12.47%	1.578%
2	1.568	157	164	179	rVB	236900	260874	13.76%	1.741%
3	2.108	322	332	363	rVB	428945	662390	34.93%	4.420%
4	2.365	410	412	416	rVB2	429	229	0.01%	0.002%
5	2.510	449	457	463	rBV3	2674	3603	0.19%	0.024%
6	2.658	501	503	509	rVB2	548	476	0.03%	0.003%
7	2.706	514	518	521	rBV3	295	290	0.02%	0.002%
8	2.751	527	532	534	rBV2	526	420	0.02%	0.003%
9	2.809	548	550	552	rVB	447	169	0.01%	0.001%
10	2.822	552	554	557	rBV3	318	159	0.01%	0.001%
11	2.889	571	575	577	rBV2	258	177	0.01%	0.001%
12	2.921	583	585	590	rVB2	209	151	0.01%	0.001%
13	2.966	594	599	600	rBV	243	183	0.01%	0.001%
14	3.111	641	644	645	rBV	321	169	0.01%	0.001%
15	3.198	667	671	672	rBV3	281	180	0.01%	0.001%
16	3.275	692	695	701	rVB	336	253	0.01%	0.002%
17	3.304	701	704	710	rBV2	346	289	0.02%	0.002%
18	3.330	710	712	714	rBV	298	133	0.01%	0.001%
19	3.362	719	722	724	rBV2	324	175	0.01%	0.001%
20	3.455	749	751	753	rBV3	311	149	0.01%	0.001%
21	3.474	755	757	760	rBV2	362	249	0.01%	0.002%
22	3.574	785	788	791	rBV2	344	232	0.01%	0.002%
23	3.593	791	794	795	rBV	355	153	0.01%	0.001%
24	3.613	798	800	803	rVB3	431	205	0.01%	0.001%
25	3.700	824	827	829	rBV2	361	221	0.01%	0.001%
26	3.725	832	835	841	rBV2	403	214	0.01%	0.001%
27	3.812	859	862	865	rBV	307	141	0.01%	0.001%
28	3.880	872	883	923	rBV	129571	381323	20.11%	2.545%
29	4.349	1012	1029	1060	rBV	304203	764224	40.30%	5.100%
30	4.728	1146	1147	1150	rVB	478	179	0.01%	0.001%
31	4.751	1150	1154	1159	rVB3	335	294	0.02%	0.002%
32	4.777	1159	1162	1168	rVB2	386	283	0.01%	0.002%
33	4.812	1168	1173	1176	rBV2	275	295	0.02%	0.002%
34	4.867	1184	1190	1193	rBV3	387	311	0.02%	0.002%
35	5.047	1228	1246	1272	rBV2	731201	1896420	100.00%	12.654%
36	5.462	1371	1375	1378	rBV2	227	196	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021221\
 Data File : VW020312.D
 Acq On : 12 Feb 2021 12:56
 Operator : SY/MD
 Sample : M1330-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
 Title : VOC Analysis

37	5.478	1378	1380	1384	rBV2	578	456	0.02%	0.003%
38	5.545	1399	1401	1403	rVB	500	217	0.01%	0.001%
39	5.561	1403	1406	1408	rBV3	375	260	0.01%	0.002%
40	5.616	1410	1423	1460	rBV	621338	1262129	66.55%	8.422%
41	5.905	1503	1513	1532	rBV3	22582	45075	2.38%	0.301%
42	6.069	1551	1564	1594	rBV	424580	866113	45.67%	5.779%
43	6.336	1645	1647	1649	rBV	520	299	0.02%	0.002%
44	6.400	1664	1667	1669	rBV2	312	177	0.01%	0.001%
45	6.413	1669	1671	1676	rVB2	452	227	0.01%	0.002%
46	6.436	1676	1678	1681	rBV3	594	359	0.02%	0.002%
47	6.452	1681	1683	1687	rVV2	478	268	0.01%	0.002%
48	6.484	1689	1693	1695	rBV3	432	376	0.02%	0.003%
49	6.622	1734	1736	1737	rBV	471	227	0.01%	0.002%
50	6.716	1763	1765	1769	rBV4	350	303	0.02%	0.002%
51	6.799	1789	1791	1796	rVB2	485	253	0.01%	0.002%
52	6.870	1810	1813	1818	rBV2	270	284	0.01%	0.002%
53	6.921	1826	1829	1833	rBV2	610	445	0.02%	0.003%
54	6.986	1838	1849	1876	rBV	225154	412616	21.76%	2.753%
55	7.317	1939	1952	1973	rBV	850893	1469692	77.50%	9.807%
56	7.555	2024	2026	2029	rBV2	683	483	0.03%	0.003%
57	7.584	2033	2035	2037	rBV	517	279	0.01%	0.002%
58	7.622	2037	2047	2070	rBV	161267	278329	14.68%	1.857%
59	7.838	2110	2114	2116	rBV	746	601	0.03%	0.004%
60	7.889	2126	2130	2134	rVB3	723	591	0.03%	0.004%
61	7.912	2134	2137	2138	rBV2	412	229	0.01%	0.002%
62	7.986	2155	2160	2164	rBV5	665	597	0.03%	0.004%
63	8.088	2181	2192	2235	rBV	434474	845533	44.59%	5.642%
64	8.545	2332	2334	2337	rBV2	528	298	0.02%	0.002%
65	8.613	2347	2355	2357	rBV5	610	660	0.03%	0.004%
66	8.741	2392	2395	2399	rBV3	371	365	0.02%	0.002%
67	8.854	2418	2430	2458	rBV	985711	1588397	83.76%	10.599%
68	9.153	2518	2523	2530	rVV2	866	1020	0.05%	0.007%
69	9.323	2573	2576	2578	rBV2	568	352	0.02%	0.002%
70	9.432	2606	2610	2613	rBV2	310	310	0.02%	0.002%
71	9.487	2624	2627	2629	rVB2	410	227	0.01%	0.002%
72	9.535	2639	2642	2648	rBV3	391	450	0.02%	0.003%
73	9.561	2648	2650	2652	rVB	415	146	0.01%	0.001%
74	9.577	2652	2655	2658	rBV3	434	336	0.02%	0.002%
75	9.828	2729	2733	2734	rBV2	298	171	0.01%	0.001%
76	9.924	2760	2763	2765	rBV	272	180	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021221\
 Data File : VV020312.D
 Acq On : 12 Feb 2021 12:56
 Operator : SY/MD
 Sample : M1330-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

77	10.040	2796	2799	2802	rBV2	464	241	0.01%	0.002%
78	10.220	2842	2855	2879	rBV	602050	930804	49.08%	6.211%
79	10.326	2885	2888	2889	rBV2	514	242	0.01%	0.002%
80	10.365	2898	2900	2904	rBV2	256	190	0.01%	0.001%
81	10.394	2907	2909	2910	rBV	383	151	0.01%	0.001%
82	10.596	2968	2972	2978	rBV2	397	447	0.02%	0.003%
83	10.680	2994	2998	3000	rBV2	376	334	0.02%	0.002%
84	10.731	3011	3014	3016	rBV2	332	179	0.01%	0.001%
85	10.921	3069	3073	3074	rBV2	519	315	0.02%	0.002%
86	11.079	3120	3122	3127	rBV2	339	232	0.01%	0.002%
87	11.175	3148	3152	3155	rBV2	820	593	0.03%	0.004%
88	11.256	3165	3177	3204	rBV	1040491	1568788	82.72%	10.468%
89	11.432	3229	3232	3236	rBV3	638	436	0.02%	0.003%
90	11.474	3243	3245	3248	rVB2	617	308	0.02%	0.002%
91	11.632	3281	3294	3318	rBV	940148	1488992	78.52%	9.936%
92	11.918	3381	3383	3385	rBV	540	292	0.02%	0.002%
93	11.998	3405	3408	3410	rBV	359	215	0.01%	0.001%
94	12.030	3415	3418	3420	rVB3	393	228	0.01%	0.002%
95	12.329	3506	3511	3512	rBV2	378	318	0.02%	0.002%
96	12.699	3624	3626	3630	rVB2	311	140	0.01%	0.001%
97	12.728	3633	3635	3637	rBV2	274	152	0.01%	0.001%
98	12.889	3683	3685	3688	rBV2	358	273	0.01%	0.002%
99	12.911	3690	3692	3697	rVB2	805	450	0.02%	0.003%
100	13.757	3952	3955	3956	rBV2	1208	660	0.03%	0.004%




Sum of corrected areas: 14986141

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021221\
Data File : VV020312.D
Acq On : 12 Feb 2021 12:56
Operator : SY/MD
Sample : M1330-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

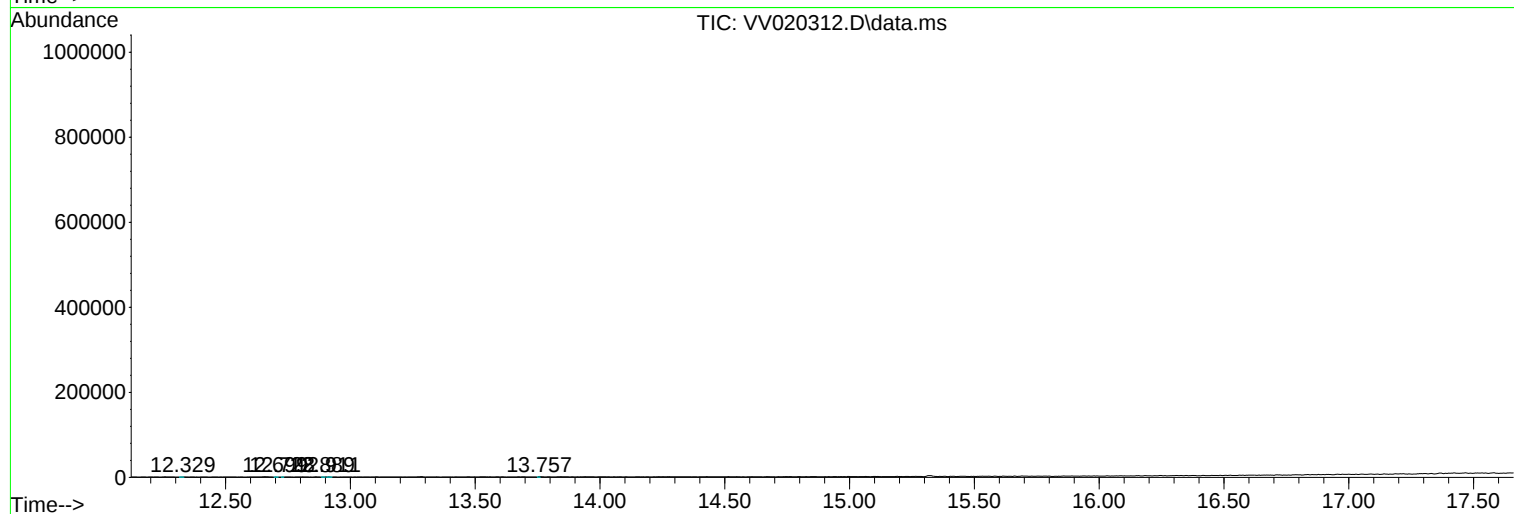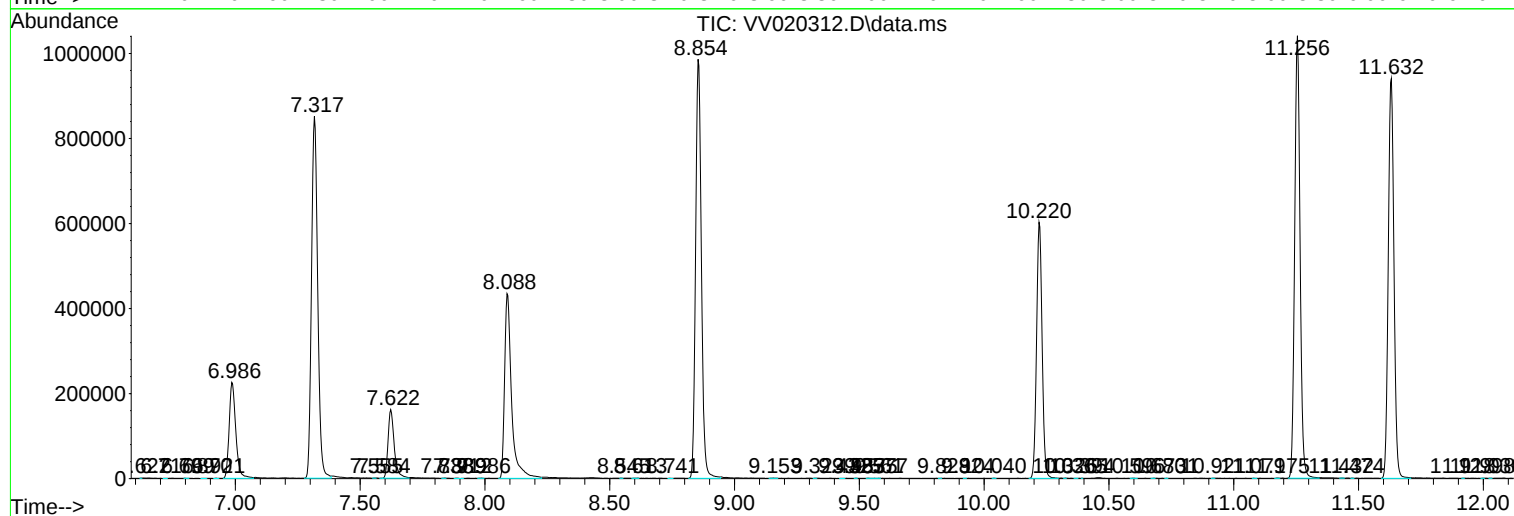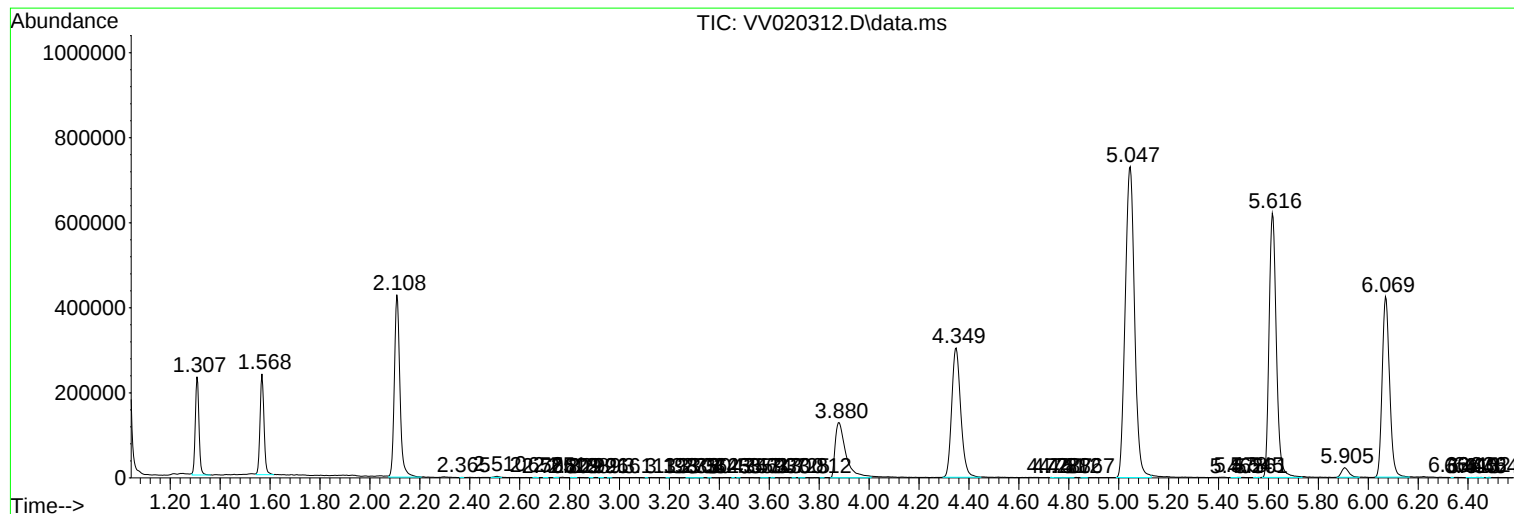

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021221\
Data File : VV020312.D
Acq On : 12 Feb 2021 12:56
Operator : SY/MD
Sample : M1330-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021221\
Data File : VV020312.D
Acq On : 12 Feb 2021 12:56
Operator : SY/MD
Sample : M1330-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
