

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021221\
 Data File : VV020314.D
 Acq On : 12 Feb 2021 16:12
 Operator : SY/MD
 Sample : VIBLK82
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK82

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

Signal : TIC: VV020314.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	98	rVB	250004	253330	13.76%	1.654%
2	1.568	158	164	177	rVB	234381	257379	13.98%	1.680%
3	2.111	323	333	361	rVB	454805	699239	37.98%	4.565%
4	2.474	444	446	450	rBV2	587	460	0.02%	0.003%
5	2.510	450	457	463	rBV7	1774	2865	0.16%	0.019%
6	2.564	469	474	477	rBV3	460	445	0.02%	0.003%
7	2.690	511	513	514	rBV3	373	135	0.01%	0.001%
8	2.725	521	524	527	rBV2	277	172	0.01%	0.001%
9	2.761	532	535	538	rBV	606	394	0.02%	0.003%
10	2.815	550	552	555	rVB2	470	188	0.01%	0.001%
11	2.838	555	559	563	rBV2	375	333	0.02%	0.002%
12	2.883	572	573	578	rVB2	340	133	0.01%	0.001%
13	2.973	597	601	604	rBV2	316	232	0.01%	0.002%
14	3.008	610	612	615	rBV2	300	152	0.01%	0.001%
15	3.031	616	619	621	rBV	337	199	0.01%	0.001%
16	3.108	641	643	646	rVB2	201	131	0.01%	0.001%
17	3.211	672	675	679	rBV	256	165	0.01%	0.001%
18	3.256	686	689	696	rBV3	486	449	0.02%	0.003%
19	3.307	701	705	708	rVV3	231	152	0.01%	0.001%
20	3.375	722	726	729	rBV	300	267	0.01%	0.002%
21	3.536	773	776	778	rBV	213	148	0.01%	0.001%
22	3.638	805	808	811	rBV3	431	182	0.01%	0.001%
23	3.687	819	823	825	rVB3	376	238	0.01%	0.002%
24	3.761	844	846	851	rBV2	384	279	0.02%	0.002%
25	3.818	861	864	866	rBV	226	164	0.01%	0.001%
26	3.835	867	869	874	rVB3	491	239	0.01%	0.002%
27	3.886	874	885	927	rBV	129270	374066	20.32%	2.442%
28	4.352	1013	1030	1060	rBV	295184	740268	40.21%	4.833%
29	4.629	1113	1116	1117	rBV2	491	258	0.01%	0.002%
30	4.809	1169	1172	1178	rBV4	595	584	0.03%	0.004%
31	4.851	1182	1185	1188	rVB2	412	238	0.01%	0.002%
32	4.960	1217	1219	1225	rVB3	324	234	0.01%	0.002%
33	4.986	1225	1227	1229	rBV3	216	141	0.01%	0.001%
34	5.050	1229	1247	1281	rBV2	715162	1840928	100.00%	12.019%
35	5.487	1380	1383	1384	rBV3	583	276	0.01%	0.002%
36	5.545	1399	1401	1404	rBV2	663	302	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021221\
 Data File : VV020314.D
 Acq On : 12 Feb 2021 16:12
 Operator : SY/MD
 Sample : VIBLK82
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK82

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
 Title : VOC Analysis

37	5.564	1404	1407	1409	rVB3	390	210	0.01%	0.001%
38	5.619	1409	1424	1455	rBV	694733	1410535	76.62%	9.209%
39	5.912	1506	1515	1532	rVB2	20186	41419	2.25%	0.270%
40	6.072	1551	1565	1586	rBV	410636	823536	44.73%	5.377%
41	6.310	1637	1639	1644	rVB4	521	345	0.02%	0.002%
42	6.439	1676	1679	1682	rBV2	304	231	0.01%	0.002%
43	6.506	1696	1700	1703	rBV3	396	321	0.02%	0.002%
44	6.545	1710	1712	1714	rBV	319	178	0.01%	0.001%
45	6.584	1721	1724	1727	rBV2	283	190	0.01%	0.001%
46	6.600	1727	1729	1734	rBV2	377	297	0.02%	0.002%
47	6.622	1734	1736	1738	rBV2	271	152	0.01%	0.001%
48	6.642	1738	1742	1745	rBV3	708	626	0.03%	0.004%
49	6.744	1771	1774	1777	rBV	480	322	0.02%	0.002%
50	6.777	1780	1784	1786	rVV3	313	240	0.01%	0.002%
51	6.789	1786	1788	1796	rVB2	448	374	0.02%	0.002%
52	6.828	1796	1800	1803	rBV3	205	168	0.01%	0.001%
53	6.847	1803	1806	1807	rBV	301	129	0.01%	0.001%
54	6.873	1811	1814	1818	rBV3	412	304	0.02%	0.002%
55	6.908	1822	1825	1827	rVB	285	157	0.01%	0.001%
56	6.989	1839	1850	1874	rBV	215591	395022	21.46%	2.579%
57	7.320	1940	1953	1983	rBV	851472	1463709	79.51%	9.556%
58	7.625	2037	2048	2073	rBV	155328	266541	14.48%	1.740%
59	7.841	2111	2115	2118	rBV5	410	371	0.02%	0.002%
60	7.870	2122	2124	2126	rVB	537	196	0.01%	0.001%
61	7.895	2126	2132	2134	rBV2	456	403	0.02%	0.003%
62	7.937	2142	2145	2147	rBV	603	366	0.02%	0.002%
63	7.950	2147	2149	2151	rVB3	494	228	0.01%	0.001%
64	8.024	2169	2172	2175	rVB	528	347	0.02%	0.002%
65	8.092	2182	2193	2230	rBV	439215	829907	45.08%	5.418%
66	8.648	2363	2366	2368	rBV2	381	241	0.01%	0.002%
67	8.677	2373	2375	2379	rVV3	297	150	0.01%	0.001%
68	8.760	2398	2401	2404	rBV2	602	325	0.02%	0.002%
69	8.802	2410	2414	2418	rVB2	492	427	0.02%	0.003%
70	8.857	2418	2431	2454	rBV	1091575	1749796	95.05%	11.424%
71	9.137	2515	2518	2519	rBV2	445	229	0.01%	0.001%
72	9.191	2532	2535	2538	rBV2	364	267	0.01%	0.002%
73	9.233	2545	2548	2550	rBV2	349	217	0.01%	0.001%
74	9.310	2570	2572	2573	rBV	360	168	0.01%	0.001%
75	9.381	2590	2594	2596	rBV2	386	235	0.01%	0.002%
76	9.420	2604	2606	2611	rBV3	300	251	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021221\
 Data File : VV020314.D
 Acq On : 12 Feb 2021 16:12
 Operator : SY/MD
 Sample : VIBLK82
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK82

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

77	9.548	2642	2646	2649	rBV2	521	464	0.03%	0.003%
78	9.706	2691	2695	2696	rBV	252	163	0.01%	0.001%
79	9.741	2703	2706	2709	rBV2	437	358	0.02%	0.002%
80	9.834	2733	2735	2740	rVB3	565	240	0.01%	0.002%
81	9.866	2740	2745	2749	rBV3	590	529	0.03%	0.003%
82	9.937	2762	2767	2770	rBV2	301	322	0.02%	0.002%
83	9.953	2770	2772	2774	rVB	352	142	0.01%	0.001%
84	10.005	2785	2788	2791	rBV2	302	178	0.01%	0.001%
85	10.079	2809	2811	2817	rBV3	322	193	0.01%	0.001%
86	10.220	2843	2855	2876	rBV	568417	892960	48.51%	5.830%
87	10.391	2904	2908	2909	rBV2	402	258	0.01%	0.002%
88	10.464	2928	2931	2933	rBV	285	227	0.01%	0.001%
89	10.587	2966	2969	2970	rBV2	335	163	0.01%	0.001%
90	10.632	2981	2983	2986	rBV	340	190	0.01%	0.001%
91	10.918	3070	3072	3075	rBV3	562	284	0.02%	0.002%
92	10.960	3081	3085	3086	rBV	396	244	0.01%	0.002%
93	11.079	3115	3122	3123	rBV2	278	294	0.02%	0.002%
94	11.175	3150	3152	3156	rBV2	505	273	0.01%	0.002%
95	11.255	3165	3177	3200	rBV	1164267	1764550	95.85%	11.520%
96	11.554	3268	3270	3274	rVB3	393	178	0.01%	0.001%
97	11.632	3281	3294	3316	rBV	942581	1462904	79.47%	9.551%
98	12.252	3483	3487	3488	rBV	579	406	0.02%	0.003%
99	15.320	4436	4441	4452	rVB7	16739	23138	1.26%	0.151%
100	15.911	4621	4625	4626	rBV4	4994	3943	0.21%	0.026%




Sum of corrected areas: 15317096

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021221\
Data File : VV020314.D
Acq On : 12 Feb 2021 16:12
Operator : SY/MD
Sample : VIBLK82
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VIBLK82

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

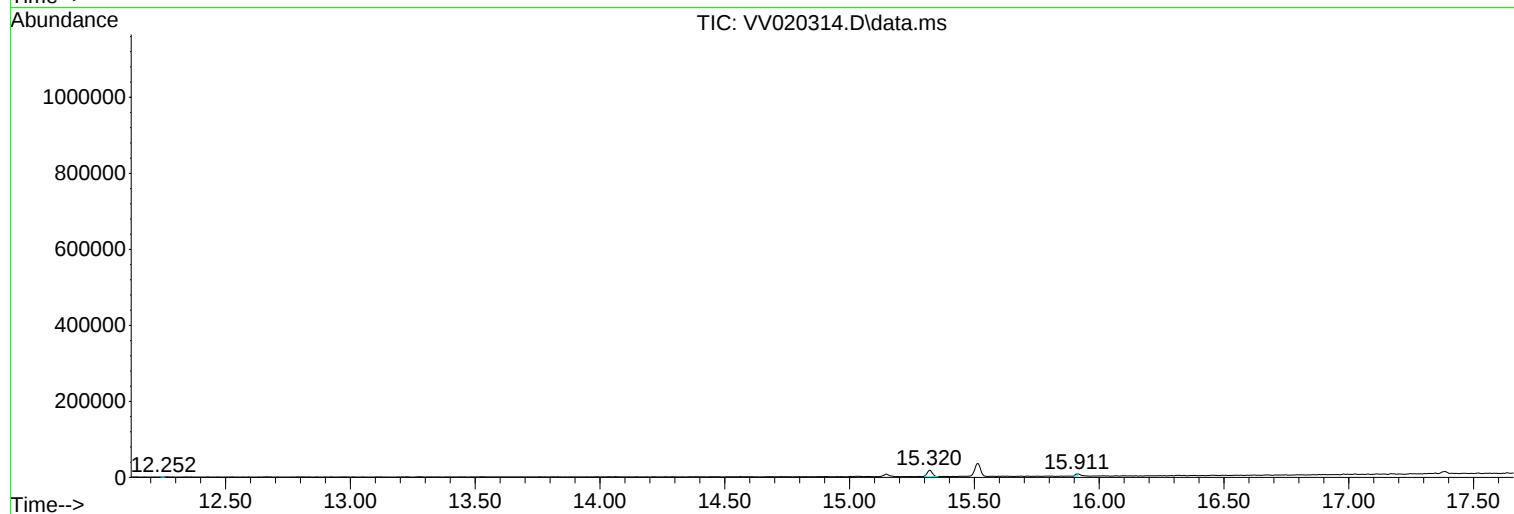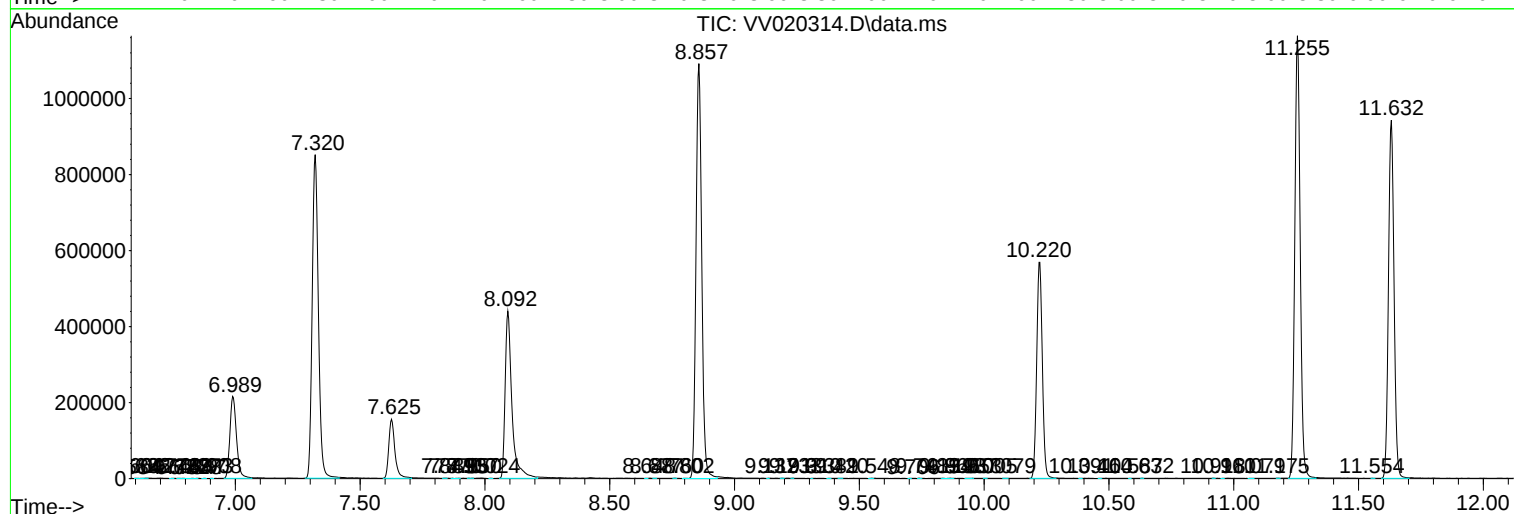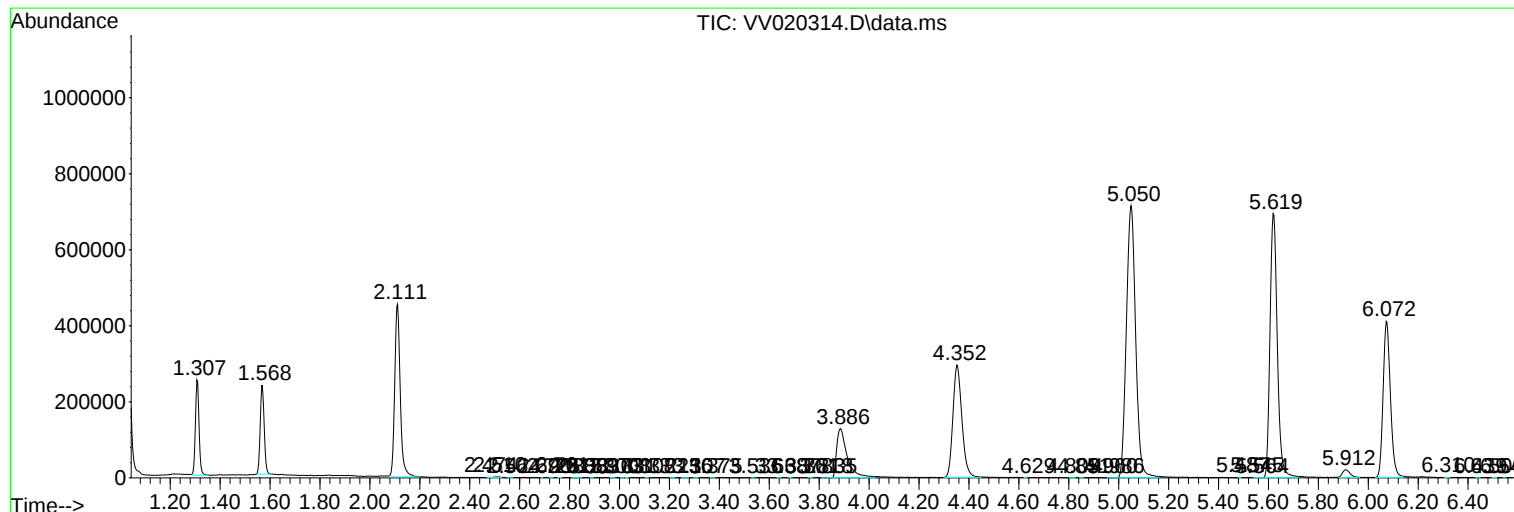

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021221\
Data File : VV020314.D
Acq On : 12 Feb 2021 16:12
Operator : SY/MD
Sample : VIBLK82
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK82

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021221\
Data File : VV020314.D
Acq On : 12 Feb 2021 16:12
Operator : SY/MD
Sample : VIBLK82
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK82

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
