
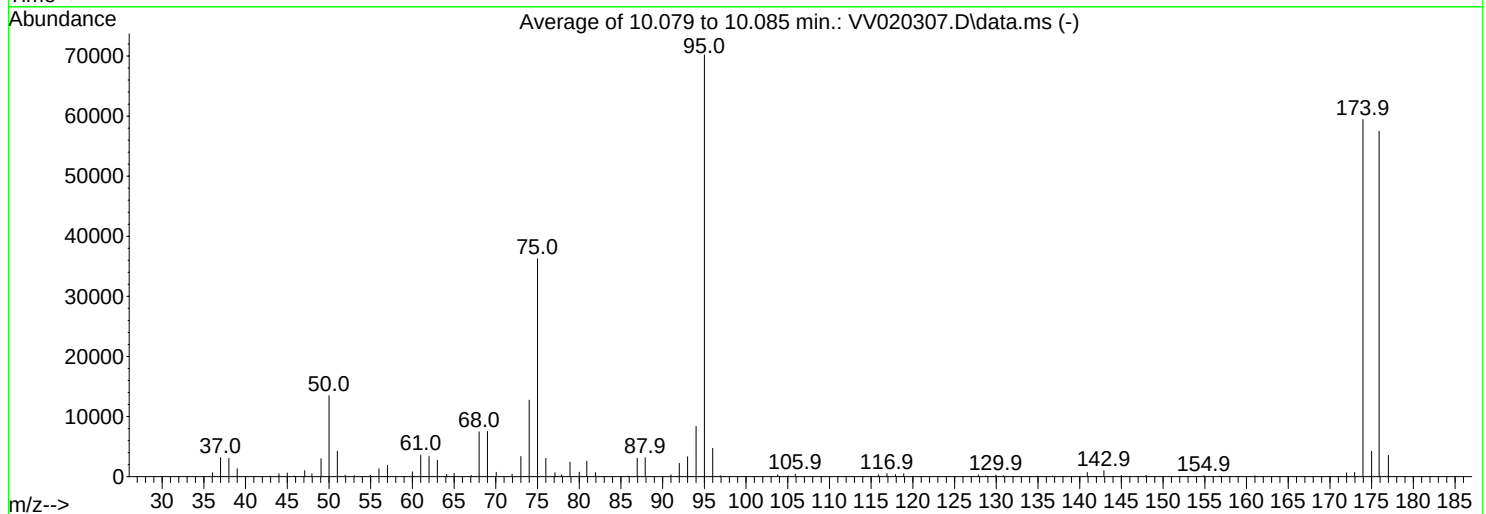


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021221\
Data File : VV020307.D
Acq On : 12 Feb 2021 08:52
Operator : SY/MD
Sample : BFB90
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB90

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Title : VOC Analysis
Last Update : Fri Feb 12 22:14:10 2021

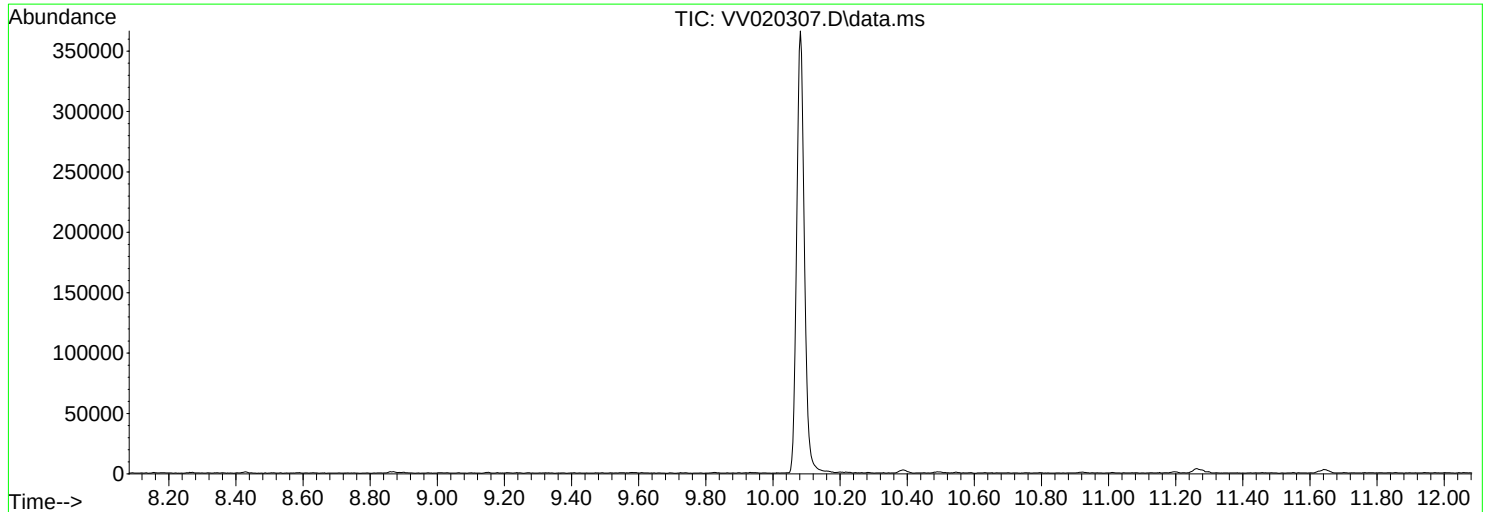

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2800

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	13476	PASS
75	95	30	80	51.7	36275	PASS
95	95	100	100	100.0	70195	PASS
96	95	5	9	6.7	4714	PASS
173	174	0.00	2	1.2	694	PASS
174	95	50	120	84.7	59432	PASS
175	174	5	9	7.1	4234	PASS
176	174	95	101	96.7	57491	PASS
177	176	5	9	6.2	3536	PASS

m/z	Abundance
36.10	628.0
37.00	3040.0
38.00	3062.0
39.00	1375.0
40.00	253.0
42.90	126.0
44.00	915.0
45.00	614.0
45.90	112.0
47.10	944.0
47.90	403.0
49.00	2937.0
50.00	13656.0
51.00	4388.0
52.00	292.0
53.10	150.0
54.90	249.0
56.00	1351.0
57.00	1807.0
58.00	113.0
60.00	727.0
61.00	3554.0
62.00	3463.0
63.00	2680.0
64.10	372.0
65.00	524.0
67.10	185.0
68.00	7478.0
69.00	7811.0
70.10	700.0
71.90	418.0
73.00	3265.0
74.00	13057.0
75.00	36296.0
76.00	3069.0
77.10	687.0
77.90	305.0
78.90	2381.0
80.00	796.0
80.90	2546.0
82.00	732.0
85.80	102.0
87.00	3076.0
87.90	2959.0
91.00	282.0
92.00	2200.0
93.00	3331.0
94.00	8224.0
95.00	69496.0
96.00	4929.0
96.90	157.0
103.80	285.0
105.10	165.0
105.90	336.0
111.10	112.0
112.80	118.0
115.80	321.0
116.90	532.0
117.90	368.0
118.90	468.0
127.90	244.0
128.80	139.0
129.90	306.0
130.80	186.0
136.70	134.0
140.90	665.0
142.90	1038.0
145.00	207.0
148.00	212.0
154.90	174.0
156.80	103.0
158.70	111.0
161.00	127.0
172.00	632.0
172.90	656.0
174.00	57128.0
175.00	4069.0
175.90	55912.0
177.00	3480.0

Instrument :
MSVOA_V
ClientSampleId :
BFB90

m/z	Abundance
36.10	676.0
37.00	3236.0
38.00	3182.0
39.00	1346.0
40.00	254.0
43.00	129.0
44.00	1045.0
45.00	598.0
45.90	120.0
47.10	1059.0
48.00	498.0
49.00	3079.0
50.00	13998.0
51.00	4332.0
52.00	278.0
53.10	166.0
55.00	259.0
56.00	1426.0
57.00	1922.0
58.00	125.0
60.00	850.0
61.00	3678.0
62.00	3456.0
63.00	2781.0
64.10	407.0
65.00	584.0
67.00	204.0
68.00	7744.0
69.00	7767.0
70.00	778.0
71.90	387.0
73.00	3483.0
74.00	13112.0
75.00	37464.0
76.00	3135.0
77.10	689.0
77.90	298.0
78.90	2525.0
80.00	762.0
80.90	2655.0
81.90	718.0
83.30	105.0
85.90	112.0
87.00	3079.0
87.90	3258.0
91.00	292.0
92.00	2299.0
93.00	3452.0
94.00	8615.0
95.00	72320.0
96.00	4884.0
96.90	169.0
103.80	329.0
105.10	146.0
105.90	411.0
111.00	107.0
115.90	318.0
116.90	500.0
117.90	318.0
118.90	480.0
127.80	289.0
128.70	133.0
129.90	308.0
130.80	166.0
134.90	124.0
136.70	145.0
140.90	725.0
142.90	1058.0
145.00	204.0
146.00	111.0
148.00	248.0
152.90	103.0
154.90	187.0
156.80	104.0
161.00	153.0
172.00	673.0
173.00	727.0
173.90	61280.0
175.00	4375.0
175.90	59496.0
177.00	3676.0

Instrument :
MSVOA_V
ClientSampleId :
BFB90

m/z	Abundance
36.00	669.0
37.00	3204.0
38.00	2983.0
39.00	1260.0
40.00	250.0
43.00	113.0
44.00	1074.0
45.00	594.0
45.80	115.0
47.10	1005.0
48.00	521.0
49.10	2902.0
50.00	12775.0
51.00	3952.0
51.90	240.0
53.00	141.0
55.00	222.0
56.00	1237.0
57.00	1917.0
60.00	867.0
61.00	3543.0
62.00	3179.0
63.00	2694.0
64.10	357.0
65.00	537.0
67.00	220.0
68.00	7184.0
69.00	7065.0
70.00	699.0
72.00	370.0
73.00	3359.0
74.00	11993.0
75.00	35064.0
76.00	2925.0
77.10	594.0
77.90	249.0
78.90	2402.0
80.00	685.0
80.90	2506.0
81.90	627.0
85.90	105.0
86.90	3016.0
87.90	3184.0
91.00	279.0
92.00	2104.0
93.00	3139.0
94.00	8249.0
95.00	68768.0
96.00	4330.0
96.90	134.0
103.80	357.0
104.80	110.0
105.90	453.0
116.00	361.0
116.90	460.0
117.90	326.0
118.90	458.0
127.80	337.0
128.80	108.0
130.00	287.0
130.90	161.0
134.90	183.0
136.80	131.0
140.90	727.0
141.80	102.0
142.90	878.0
145.00	165.0
146.00	107.0
147.90	266.0
154.90	190.0
156.80	120.0
161.00	131.0
172.00	644.0
173.00	699.0
173.90	59888.0
175.00	4258.0
175.90	57064.0
177.00	3453.0

Instrument :
MSVOA_V
ClientSampleId :
BFB90

m/z	Abundance
39.90	236.0
41.20	132.0
44.00	537.0

Instrument :
MSVOA_V
ClientSampleId :
BFB90