

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021224\
 Data File : VW034132.D
 Acq On : 12 Feb 2024 12:11
 Operator : SY/MD
 Sample : P1402-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG9

Quant Time: Feb 13 00:45:55 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Feb 13 00:43:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	78457	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	73526	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	38927	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	26012	4.281	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.600%
7) Chloroethane-d5	1.535	69	22662	4.258	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.200%
11) 1,1-Dichloroethene-d2	2.060	65	12448	4.248	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	85.000%
20) 2-Butanone-d5	3.805	46	44748	43.849	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	87.700%
24) Chloroform-d	4.249	84	48869	4.426	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.600%
26) 1,2-Dichloroethane-d4	4.947	65	24334	4.716	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.400%
32) Benzene-d6	4.963	84	93593	4.243	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.800%
36) 1,2-Dichloropropane-d6	5.992	67	25372	4.115	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	82.200%
41) Toluene-d8	7.243	98	86121	4.248	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.000%
43) trans-1,3-Dichloroprop...	7.561	79	10297	4.422	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.400%
46) 2-Hexanone-d5	8.027	63	34448	41.444	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	82.880%
56) 1,1,2,2-Tetrachloroeth...	10.153	84	16162	4.323	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.400%
66) 1,2-Dichlorobenzene-d4	11.561	152	30578	4.319	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	86.400%
Target Compounds					Qvalue	
13) Acetone	2.130	43	7878	10.176	ug/L	# 44


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021224\
Data File : VV034132.D
Acq On : 12 Feb 2024 12:11
Operator : SY/MD
Sample : P1402-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG9

Quant Time: Feb 13 00:45:55 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Feb 13 00:43:48 2024
Response via : Initial Calibration

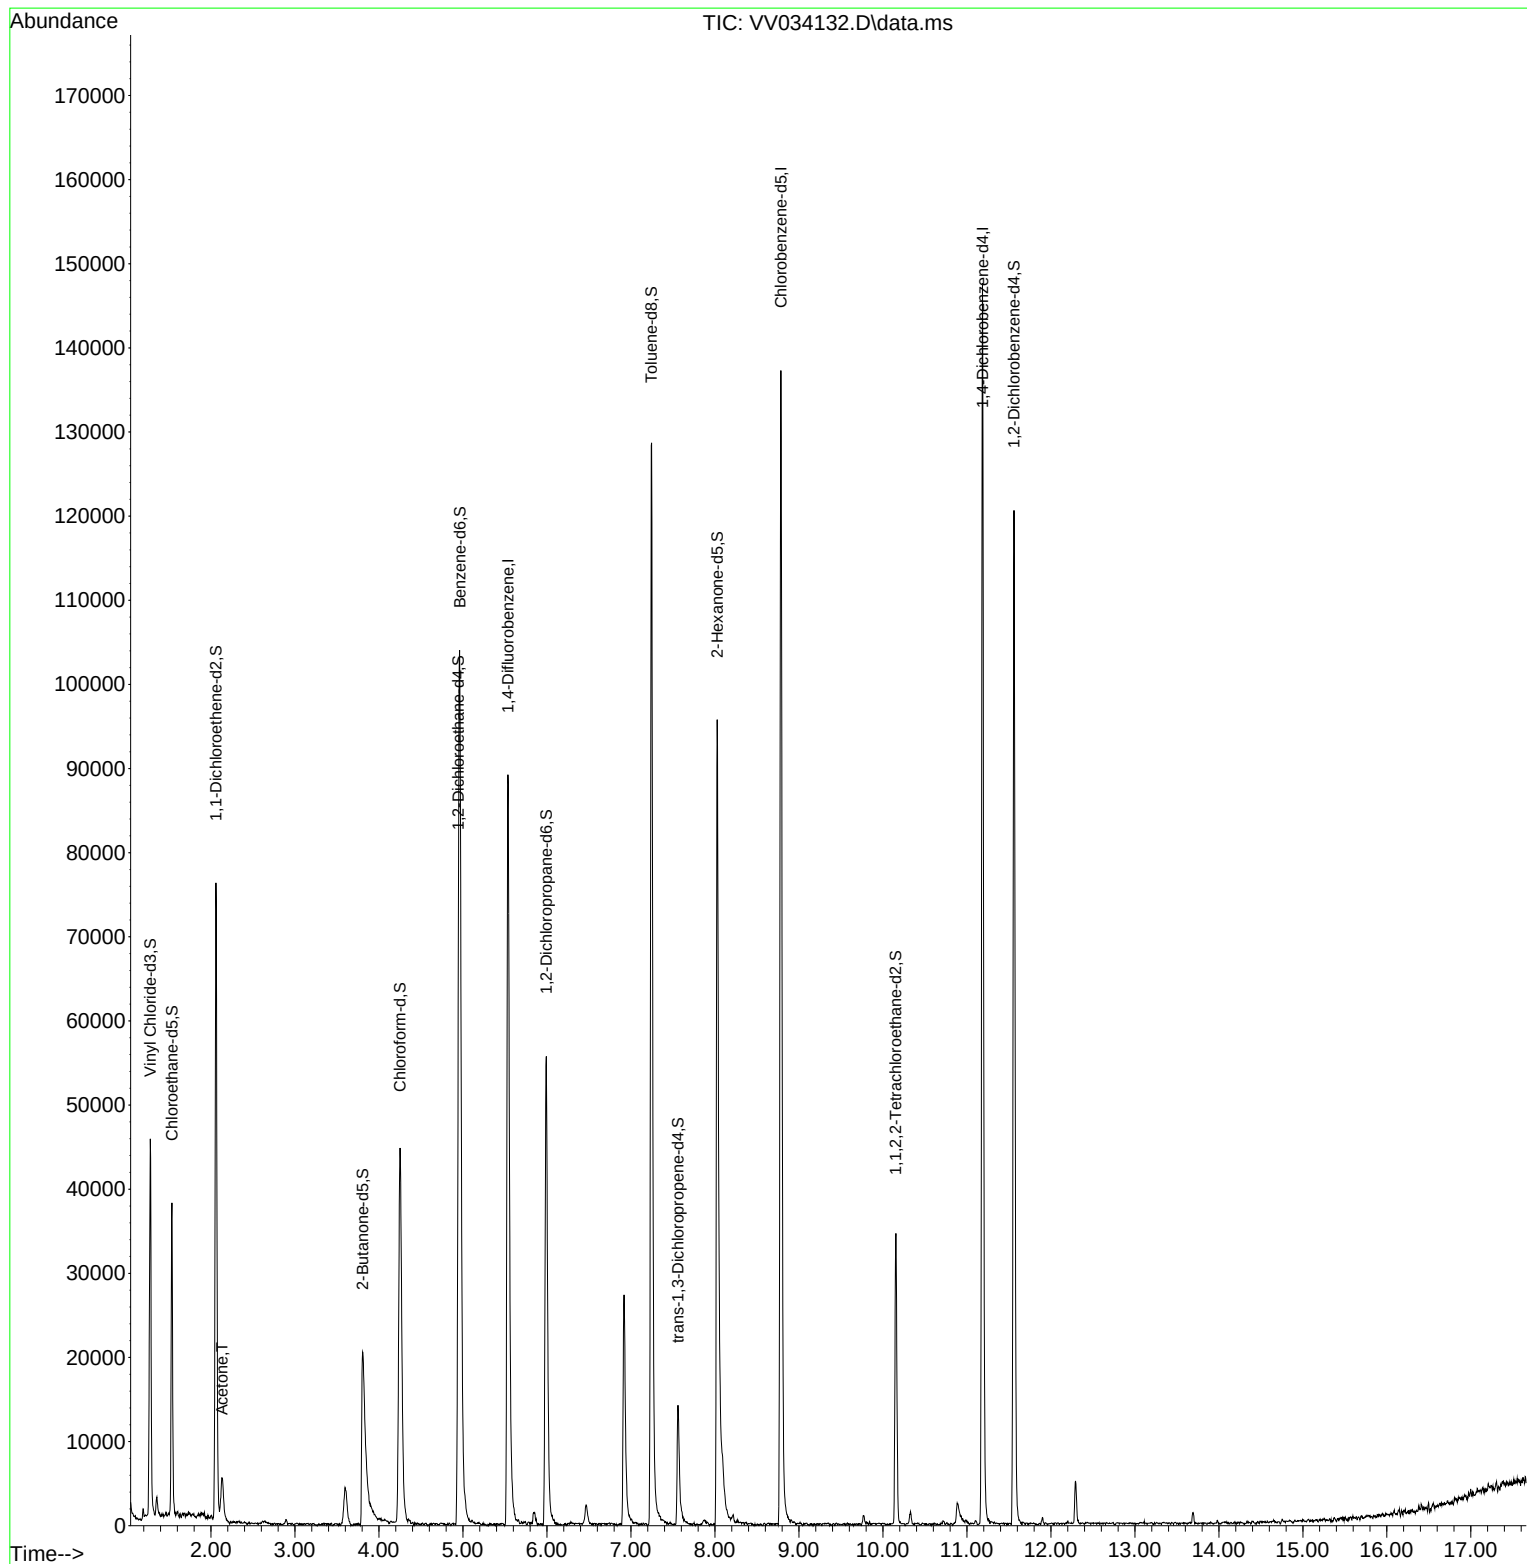

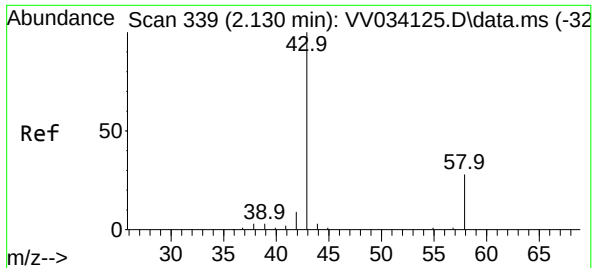

#13
 Acetone
 Concen: 10.176 ug/L
 RT: 2.130 min Scan# 31
 Delta R.T. 0.000 min
 Lab File: VV034132.D
 Acq: 12 Feb 2024 12:11

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG9

Tgt Ion: 43 Resp: 7878
 Ion Ratio Lower Upper
 43 100
 58 26.3 0.0 13.8#

