

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021224\
 Data File : VW034140.D
 Acq On : 12 Feb 2024 15:20
 Operator : SY/MD
 Sample : P1455-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COAH0

Quant Time: Feb 13 00:47:48 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Feb 13 00:43:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	74667	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	70202	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	37144	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	23197	4.011	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.200%
7) Chloroethane-d5	1.532	69	20846	4.116	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	82.400%
11) 1,1-Dichloroethene-d2	2.060	65	11391	4.085	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	81.600%
20) 2-Butanone-d5	3.802	46	39696	40.873	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	81.740%
24) Chloroform-d	4.253	84	46249	4.401	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.000%
26) 1,2-Dichloroethane-d4	4.947	65	23505	4.787	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.800%
32) Benzene-d6	4.963	84	86972	4.129	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.600%
36) 1,2-Dichloropropane-d6	5.992	67	25010	4.248	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	85.000%
41) Toluene-d8	7.246	98	80848	4.177	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.600%
43) trans-1,3-Dichloroprop...	7.561	79	9615	4.325	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.400%
46) 2-Hexanone-d5	8.027	63	34741	43.776	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.560%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	16228	4.547	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.000%
66) 1,2-Dichlorobenzene-d4	11.561	152	30185	4.468	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	89.400%
Target Compounds						
13) Acetone	2.127	43	5860	7.953	ug/L	Qvalue # 39


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021224\
Data File : VV034140.D
Acq On : 12 Feb 2024 15:20
Operator : SY/MD
Sample : P1455-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COAH0

Quant Time: Feb 13 00:47:48 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Feb 13 00:43:48 2024
Response via : Initial Calibration

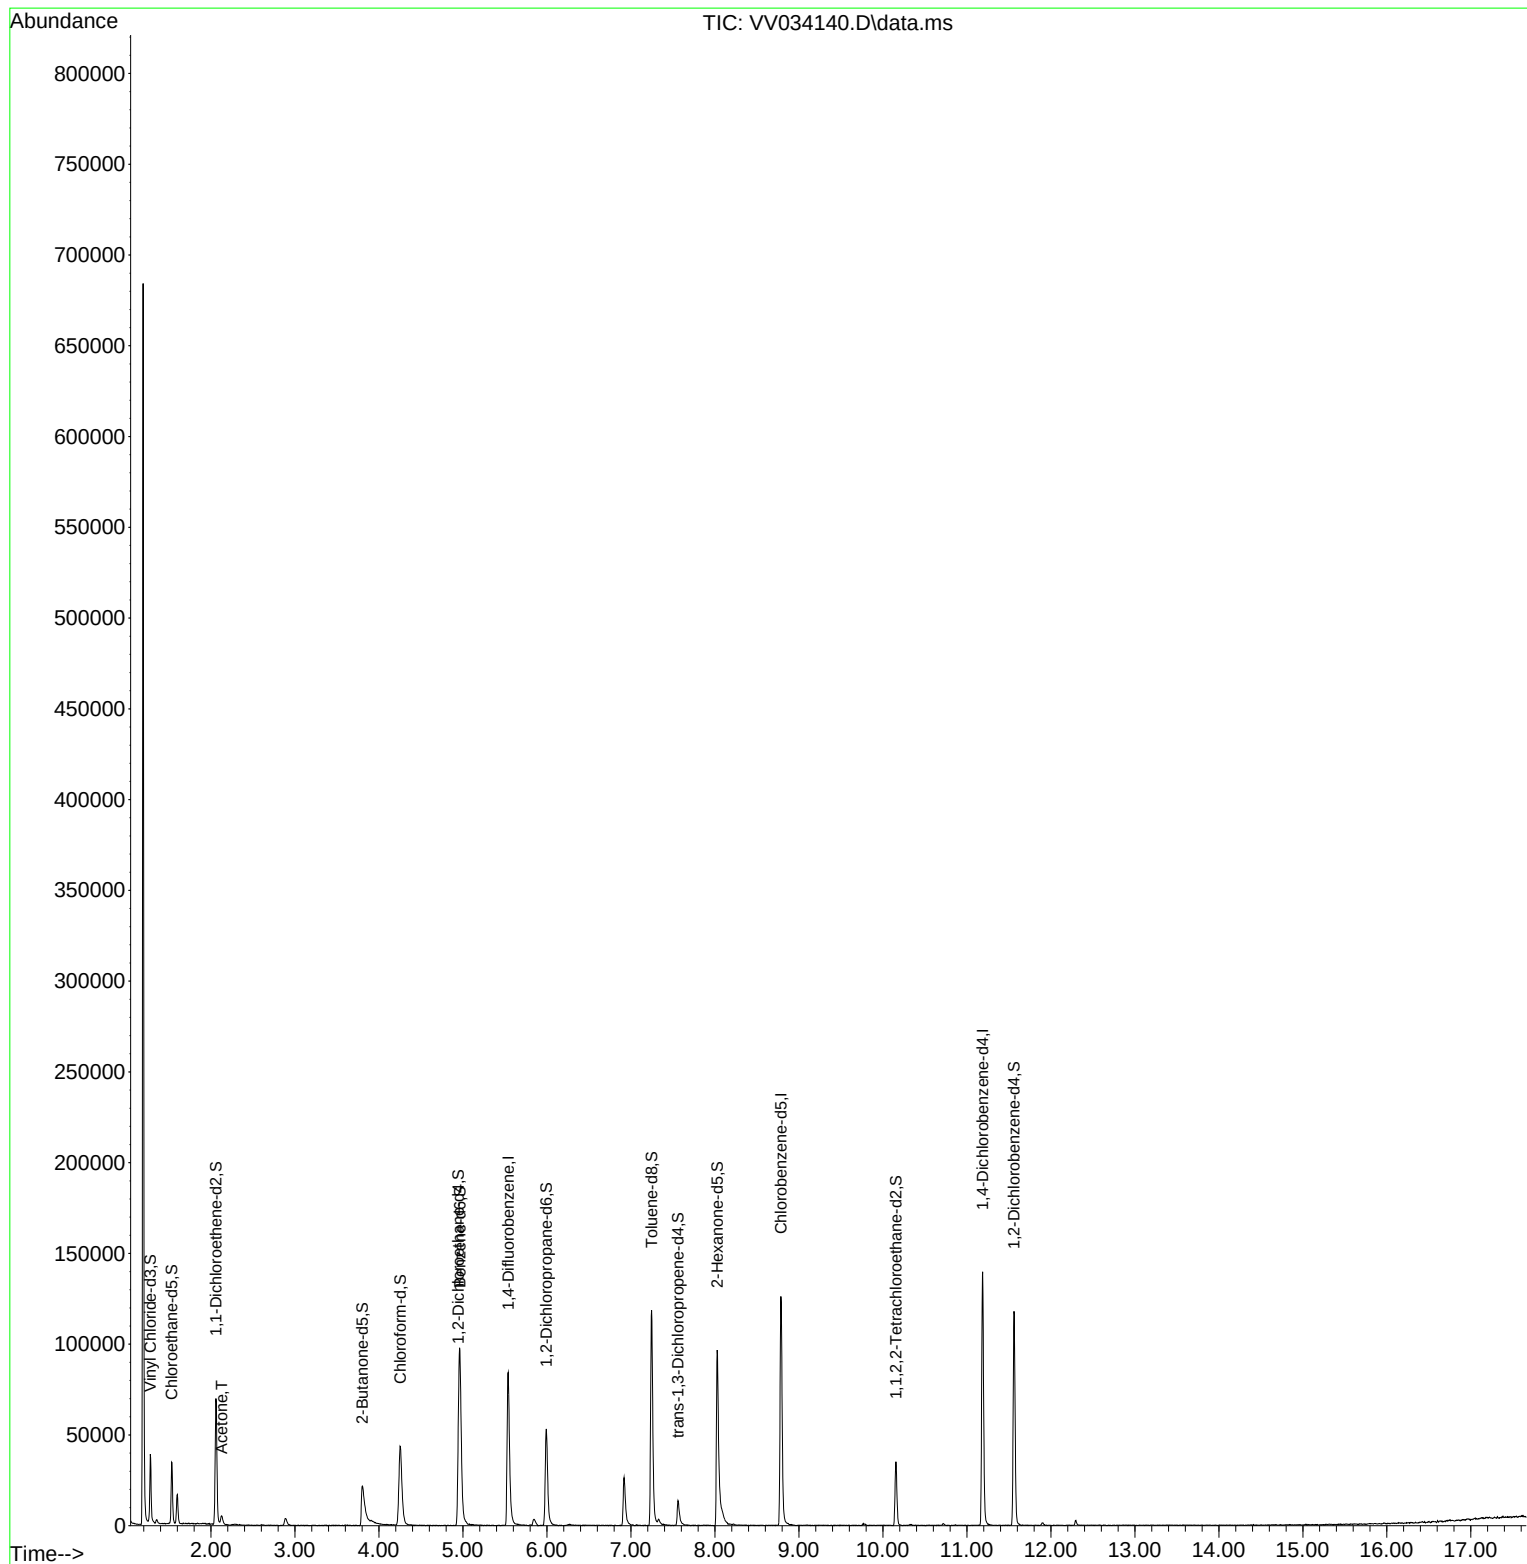

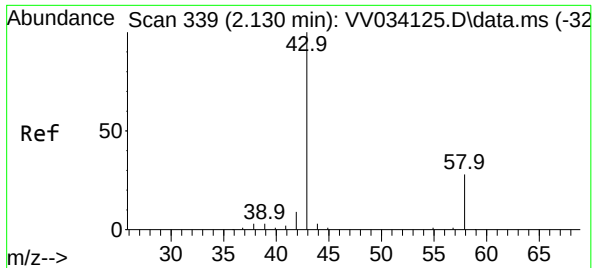

#13
 Acetone
 Concen: 7.953 ug/L
 RT: 2.127 min Scan# 31
 Delta R.T. -0.003 min
 Lab File: VV034140.D
 Acq: 12 Feb 2024 15:20

Instrument :
 MSVOA_V
 ClientSampleId :
 COAH0

Tgt Ion: 43 Resp: 5860
 Ion Ratio Lower Upper
 43 100
 58 27.9 0.0 13.8#

