

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021224\
 Data File : VW034141.D
 Acq On : 12 Feb 2024 15:44
 Operator : SY/MD
 Sample : VIBLK321
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK321

Quant Time: Feb 13 00:48:01 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Feb 13 00:43:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.538	114	72628	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	69249	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	36226	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	25872	4.600	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	92.000%	
7) Chloroethane-d5	1.532	69	21445	4.353	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	87.000%	
11) 1,1-Dichloroethene-d2	2.060	65	11904	4.388	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	87.800%	
20) 2-Butanone-d5	3.809	46	41287	43.705	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	87.400%	
24) Chloroform-d	4.252	84	47733	4.670	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	93.400%	
26) 1,2-Dichloroethane-d4	4.947	65	24692	5.169	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	103.400%	
32) Benzene-d6	4.963	84	90603	4.361	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	87.200%	
36) 1,2-Dichloropropane-d6	5.992	67	25698	4.425	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	88.400%	
41) Toluene-d8	7.246	98	83919	4.395	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	87.800%	
43) trans-1,3-Dichloroprop...	7.564	79	9866	4.499	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	90.000%	
46) 2-Hexanone-d5	8.027	63	35317	45.114	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	90.220%	
56) 1,1,2,2-Tetrachloroeth...	10.156	84	16248	4.615	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	92.200%	
66) 1,2-Dichlorobenzene-d4	11.561	152	30893	4.689	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	93.800%	
Target Compounds						
					Qvalue	
16) Methylene chloride	2.449	84	854	0.175	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021224\
Data File : VV034141.D
Acq On : 12 Feb 2024 15:44
Operator : SY/MD
Sample : VIBLK321
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK321

Quant Time: Feb 13 00:48:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Feb 13 00:43:48 2024
Response via : Initial Calibration

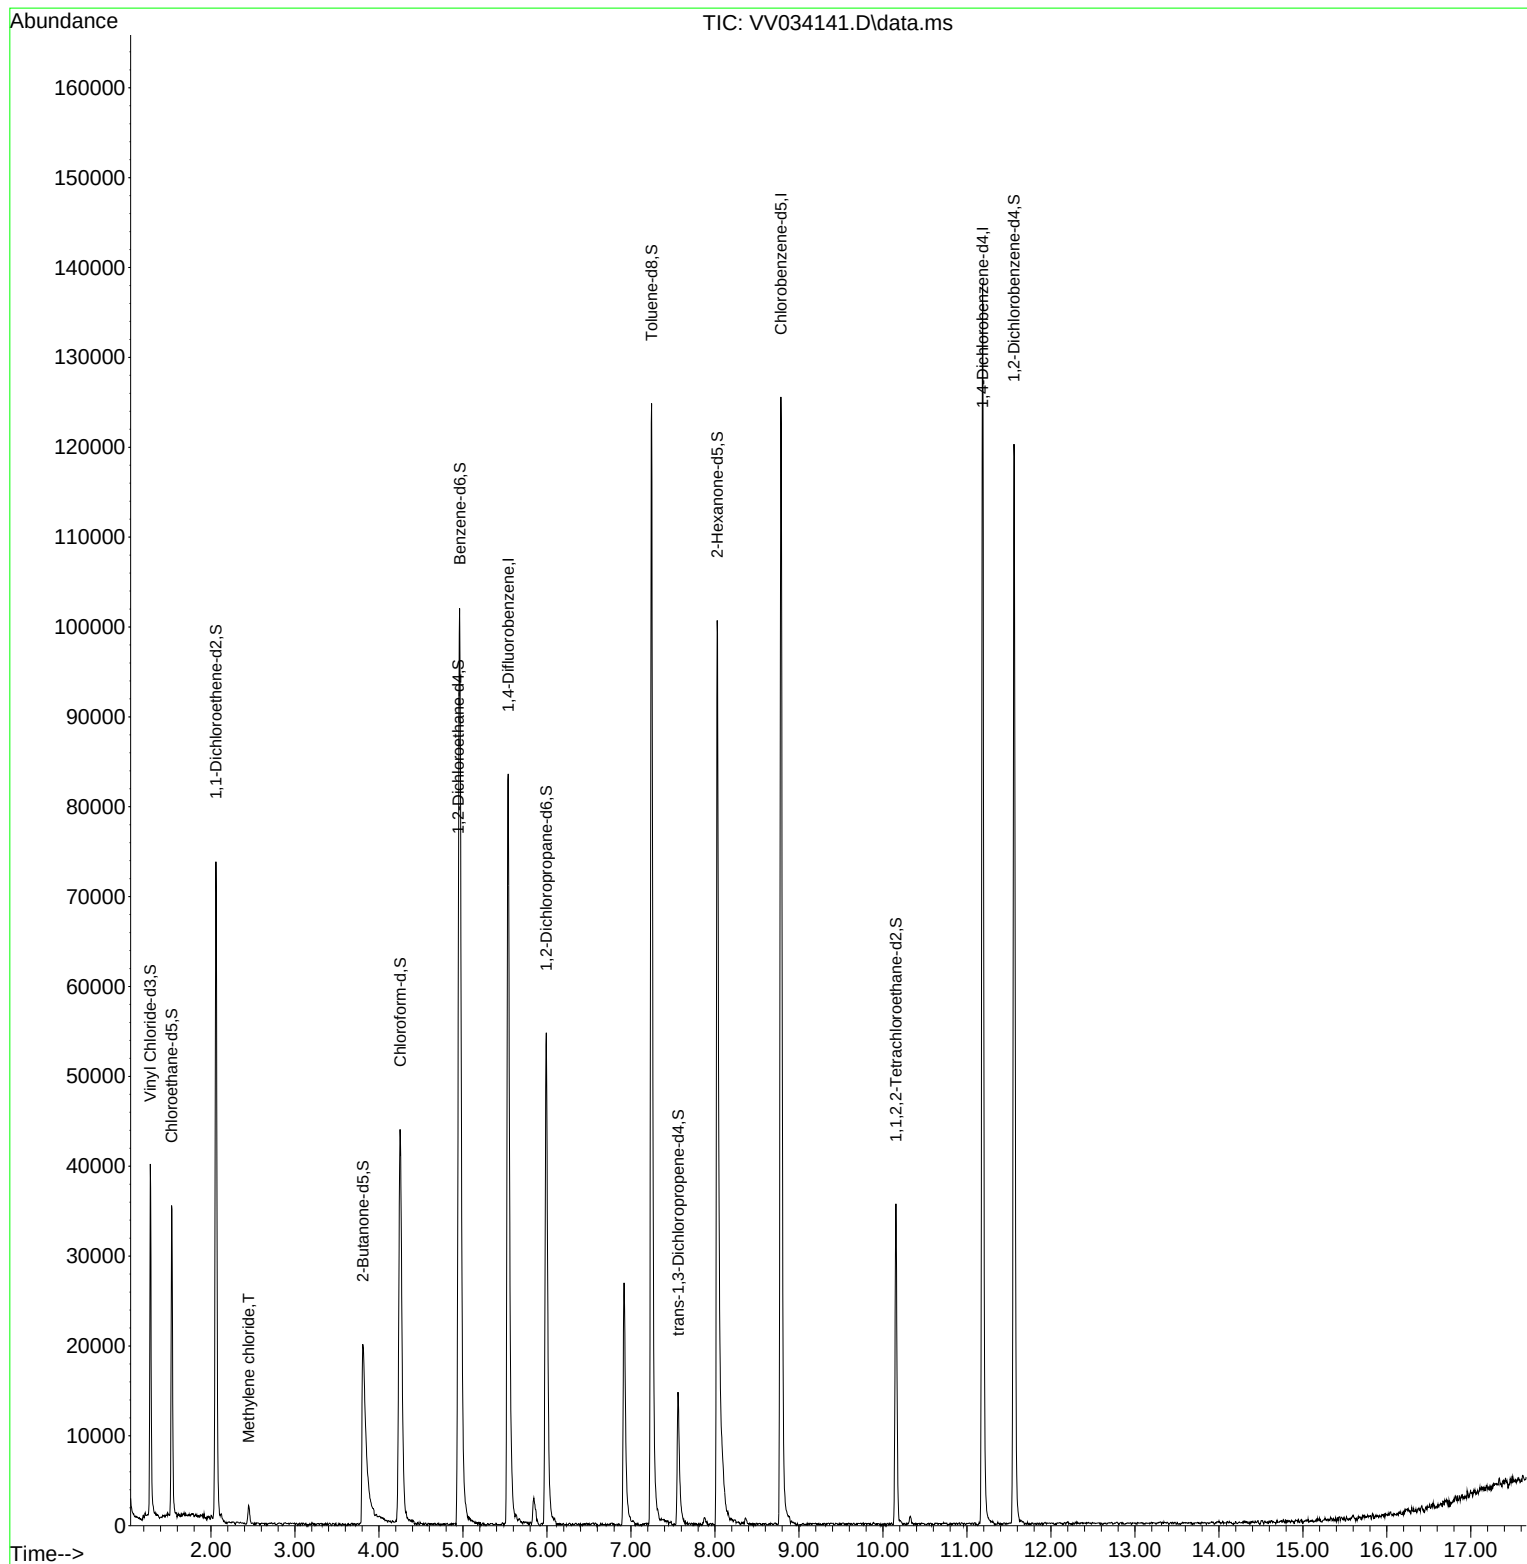

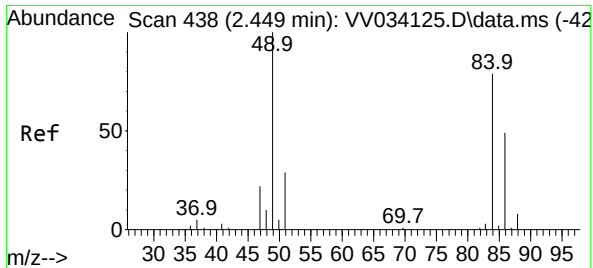

#16
Methylene chloride
Concen: 0.175 ug/L
RT: 2.449 min Scan# 41
Delta R.T. -0.000 min
Lab File: VV034141.D
Acq: 12 Feb 2024 15:44

Instrument :
MSVOA_V
ClientSampleId :
VIBLK321

Tgt Ion:	84	Resp:	854
Ion	Ratio	Lower	Upper
84	100		
86	59.0	44.7	83.1
49	116.4	93.7	173.9

