

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021224\
 Data File : VV034139.D
 Acq On : 12 Feb 2024 14:57
 Operator : SY/MD
 Sample : P1455-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV034139.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	67	75	91	rBV	36133	39527	16.46%	1.665%
2	1.532	146	153	164	rBV	32343	38656	16.10%	1.628%
3	2.059	306	317	331	rBV	68624	101993	42.49%	4.295%
4	3.802	850	859	886	rBV2	22845	70173	29.23%	2.955%
5	4.252	984	999	1027	rBV2	41984	114706	47.78%	4.830%
6	4.741	1137	1151	1167	rBV4	9686	23834	9.93%	1.004%
7	4.960	1205	1219	1247	rBV2	95079	240068	100.00%	10.110%
8	5.538	1388	1399	1426	rBV	84410	175432	73.08%	7.388%
9	5.837	1481	1492	1520	rBV	72062	146547	61.04%	6.171%
10	5.992	1528	1540	1558	rBV2	51988	107467	44.77%	4.526%
11	6.918	1820	1828	1848	rBV	25633	49749	20.72%	2.095%
12	7.246	1919	1930	1964	rBV	118635	213666	89.00%	8.998%
13	7.561	2020	2028	2055	rVB2	12819	26247	10.93%	1.105%
14	7.908	2125	2136	2152	rBV2	90387	154637	64.41%	6.512%
15	8.027	2165	2173	2213	rBV	95423	195735	81.53%	8.243%
16	8.786	2399	2409	2434	rBV	130624	216862	90.33%	9.132%
17	10.156	2825	2835	2853	rBV2	33238	53948	22.47%	2.272%
18	11.188	3145	3156	3181	rBV	138705	221582	92.30%	9.331%
19	11.561	3261	3272	3293	rBV	117200	183812	76.57%	7.741%




Sum of corrected areas: 2374641

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021224\
Data File : VV034139.D
Acq On : 12 Feb 2024 14:57
Operator : SY/MD
Sample : P1455-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

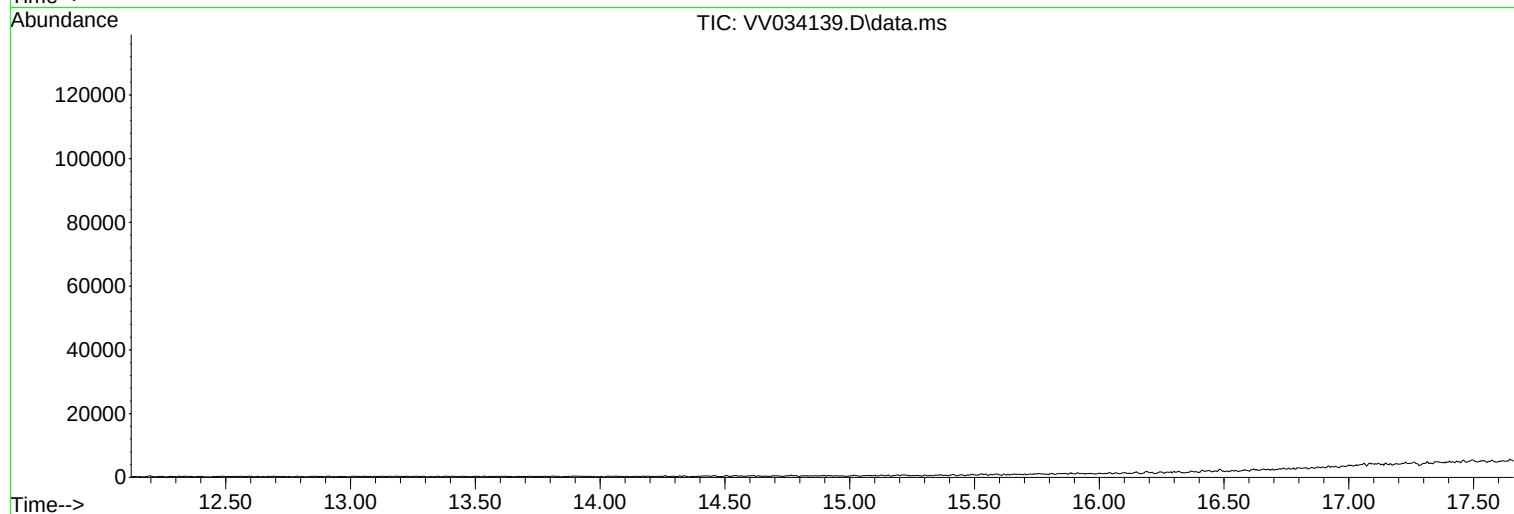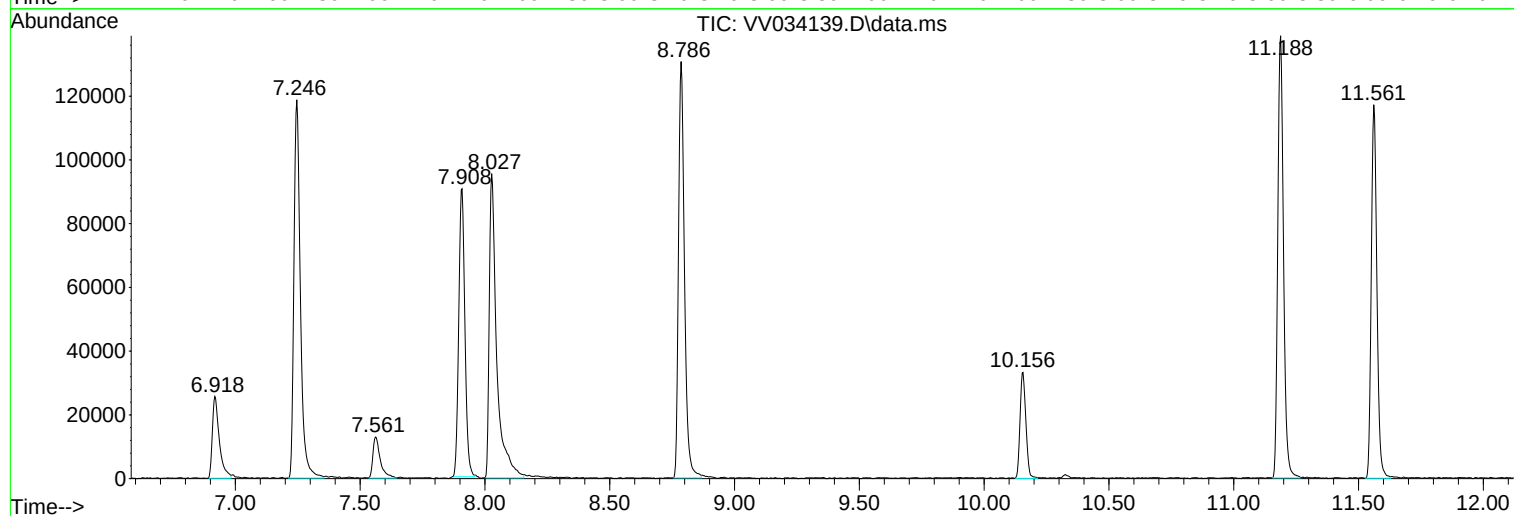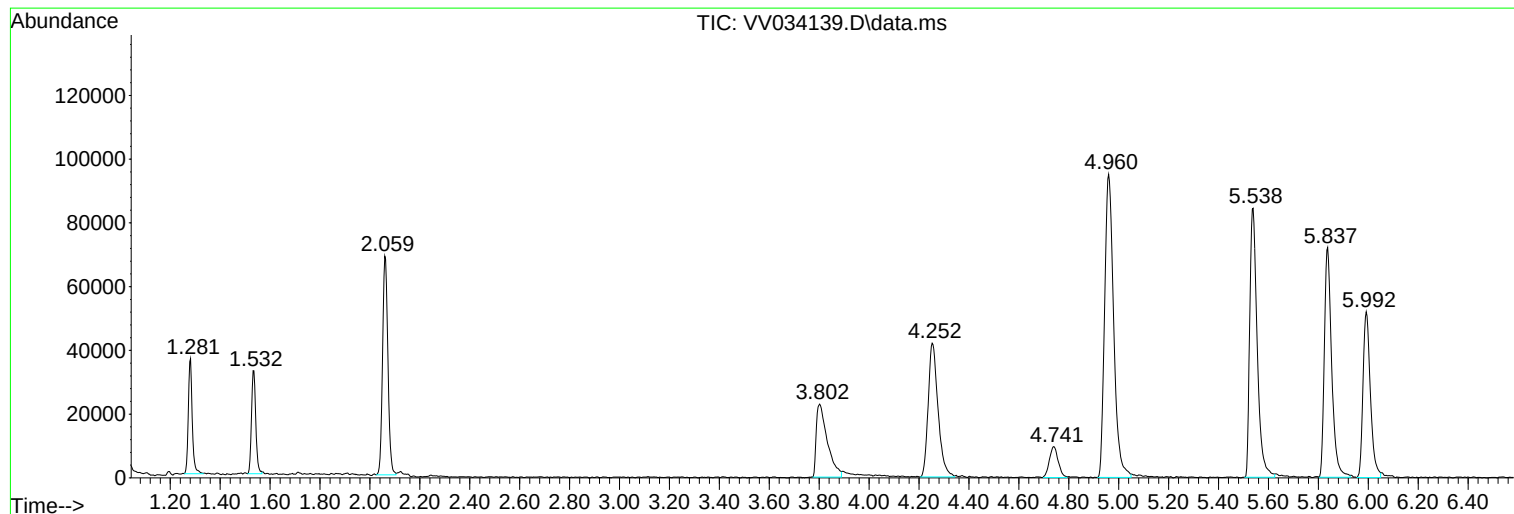

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021224\
Data File : VV034139.D
Acq On : 12 Feb 2024 14:57
Operator : SY/MD
Sample : P1455-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021224\
Data File : VV034139.D
Acq On : 12 Feb 2024 14:57
Operator : SY/MD
Sample : P1455-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc