


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021224\
Data File : VV034124.D
Acq On : 12 Feb 2024 08:29
Operator : SY/MD
Sample : BFB250
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB250

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Feb 14 01:41:00 2024

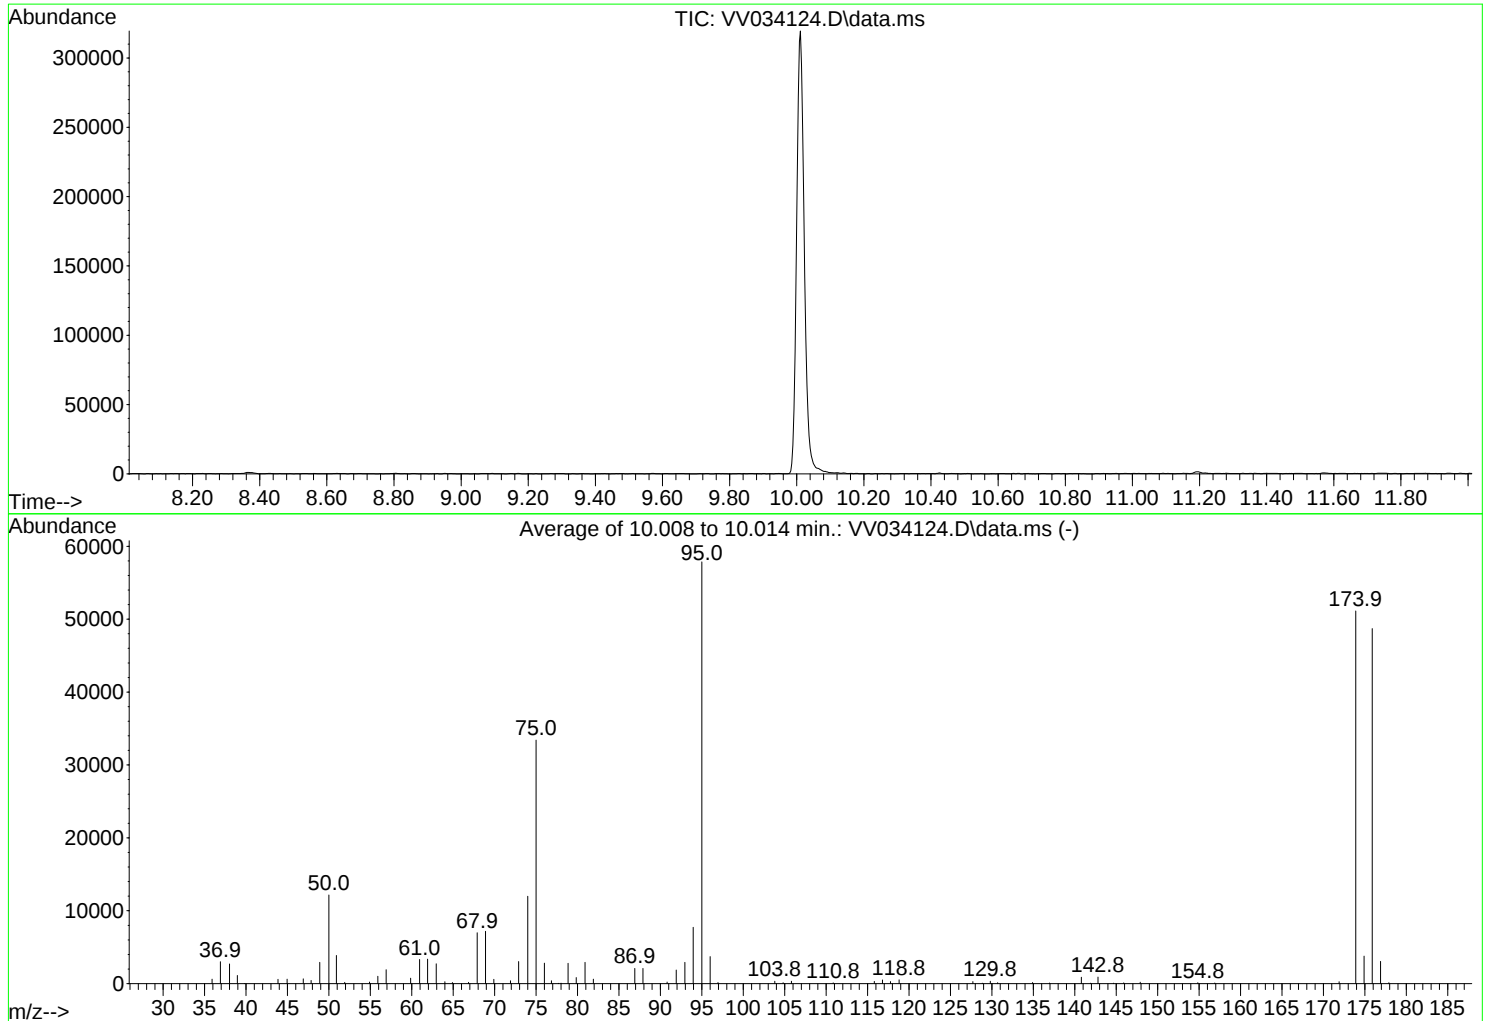

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	12159	PASS
75	95	30	80	57.8	33419	PASS
95	95	100	100	100.0	57867	PASS
96	95	5	9	6.4	3711	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	88.3	51125	PASS
175	174	5	9	7.4	3766	PASS
176	174	95	105	95.3	48709	PASS
177	176	5	10	6.3	3053	PASS

m/z	Abundance
39.90	142.0

Instrument :
MSVOA_V
ClientSampleId :
BFB250

m/z	Abundance
35.90	666.0
36.90	3192.0
38.00	2749.0
38.90	1165.0
39.80	171.0
43.80	594.0
45.00	626.0
46.90	608.0
47.90	439.0
48.90	2984.0
50.00	12297.0
50.90	3872.0
51.90	208.0
54.90	220.0
55.90	1061.0
56.90	1920.0
59.80	802.0
60.90	3424.0
61.90	3408.0
63.00	2801.0
64.00	296.0
64.90	189.0
66.80	188.0
67.90	7125.0
68.90	7589.0
69.90	564.0
71.90	385.0
72.90	3134.0
74.00	12314.0
75.00	34120.0
76.00	2852.0
76.90	423.0
78.90	2737.0
79.90	817.0
80.90	2930.0
81.90	657.0
86.90	2137.0
87.90	2224.0
90.70	243.0
91.90	1944.0
93.00	2974.0
94.00	7770.0
95.00	58704.0
96.00	3888.0
96.90	178.0
103.80	381.0
104.80	122.0
105.80	367.0
110.80	121.0
115.80	270.0
116.80	535.0
117.70	286.0
118.80	460.0
127.70	300.0
128.80	102.0
129.80	297.0
130.70	114.0
134.90	148.0
140.80	850.0
142.80	816.0
147.90	189.0
154.90	145.0
172.00	264.0
173.90	51008.0
174.90	3855.0
175.90	48400.0
176.90	3113.0
177.90	118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB250

m/z	Abundance
35.90	637.0
36.90	3152.0
38.00	2765.0
38.90	1144.0
39.80	166.0
43.80	623.0
45.00	627.0
46.90	688.0
47.80	438.0
48.90	3027.0
50.00	12553.0
50.90	3978.0
51.90	187.0
54.90	224.0
55.90	1072.0
56.90	1950.0
59.90	775.0
60.90	3422.0
61.90	3448.0
63.00	2818.0
64.00	272.0
64.90	158.0
66.80	187.0
67.90	7236.0
68.90	7359.0
69.90	623.0
71.90	398.0
72.90	3123.0
74.00	12371.0
75.00	34576.0
76.00	2897.0
76.90	425.0
78.00	176.0
78.90	2871.0
79.90	858.0
80.90	3044.0
81.90	639.0
86.90	2131.0
87.90	2174.0
90.80	216.0
91.90	1917.0
93.00	3013.0
94.00	8046.0
95.00	59856.0
96.00	3851.0
96.90	158.0
103.80	337.0
104.80	135.0
105.80	331.0
110.80	124.0
115.80	320.0
116.80	526.0
117.80	280.0
118.80	552.0
127.70	299.0
128.90	107.0
129.80	342.0
130.70	146.0
134.90	166.0
137.00	117.0
140.80	916.0
141.90	106.0
142.80	953.0
144.70	100.0
145.90	145.0
147.90	208.0
154.80	135.0
156.90	119.0
171.90	275.0
173.90	52864.0
174.90	3894.0
175.90	50376.0
176.90	3177.0
177.90	142.0

Instrument :
MSVOA_V
ClientSampleId :
BFB250

m/z	Abundance
35.90	551.0
36.90	2689.0
38.00	2586.0
39.00	1024.0
39.80	139.0
43.90	559.0
44.90	566.0
46.90	711.0
47.80	415.0
48.90	2764.0
50.00	11627.0
50.90	3714.0
51.90	147.0
54.90	192.0
55.90	916.0
56.90	1860.0
59.90	679.0
61.00	3096.0
61.90	3216.0
62.90	2538.0
64.00	224.0
64.90	122.0
66.90	169.0
67.90	6618.0
68.90	6557.0
69.90	601.0
71.90	384.0
72.90	2802.0
74.00	11292.0
75.00	31560.0
76.00	2656.0
76.80	361.0
77.70	164.0
78.80	2746.0
79.80	809.0
80.90	2799.0
81.90	562.0
86.90	2019.0
87.90	1883.0
90.90	214.0
91.90	1740.0
92.90	2751.0
93.90	7387.0
95.00	55040.0
96.00	3393.0
97.00	117.0
103.80	296.0
104.80	117.0
105.80	274.0
110.90	111.0
115.80	313.0
116.80	488.0
117.80	266.0
118.80	543.0
127.70	267.0
129.80	326.0
130.70	143.0
134.90	169.0
136.90	121.0
140.80	858.0
141.90	111.0
142.80	960.0
144.70	106.0
145.90	160.0
147.90	206.0
154.80	129.0
156.90	148.0
171.80	256.0
173.90	49504.0
174.90	3548.0
175.90	47352.0
176.90	2869.0
177.90	127.0

Instrument :
MSVOA_V
ClientSampleId :
BFB250