

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021521\
Data File : VW020322.D
Acq On : 15 Feb 2021 12:40
Operator : SY/MD
Sample : M1370-12ME
Misc : 4.75g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBGY8ME

Manual Integrations
APPROVED

MMDadoda
2/17/2021 10:34:59 AM

Quant Time: Feb 16 00:33:25 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis
Qlast Update : Tue Feb 16 00:32:19 2021
Response via : Initial Calibration

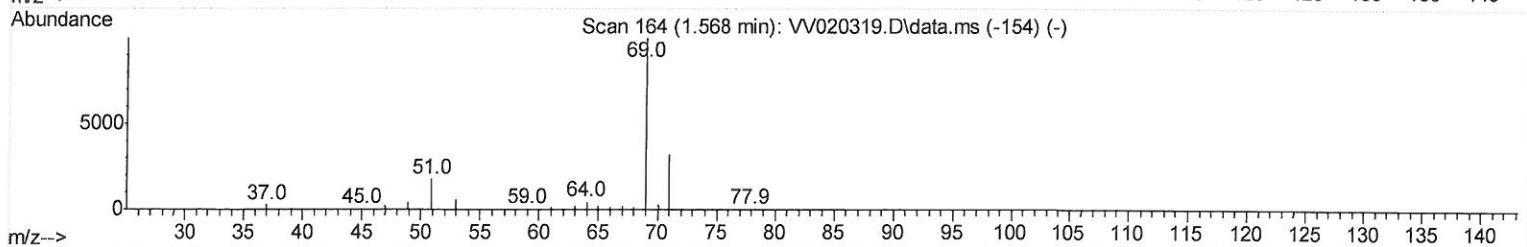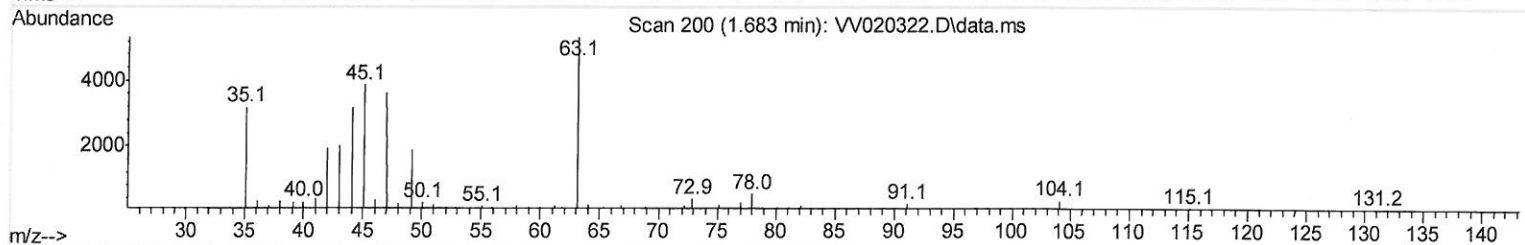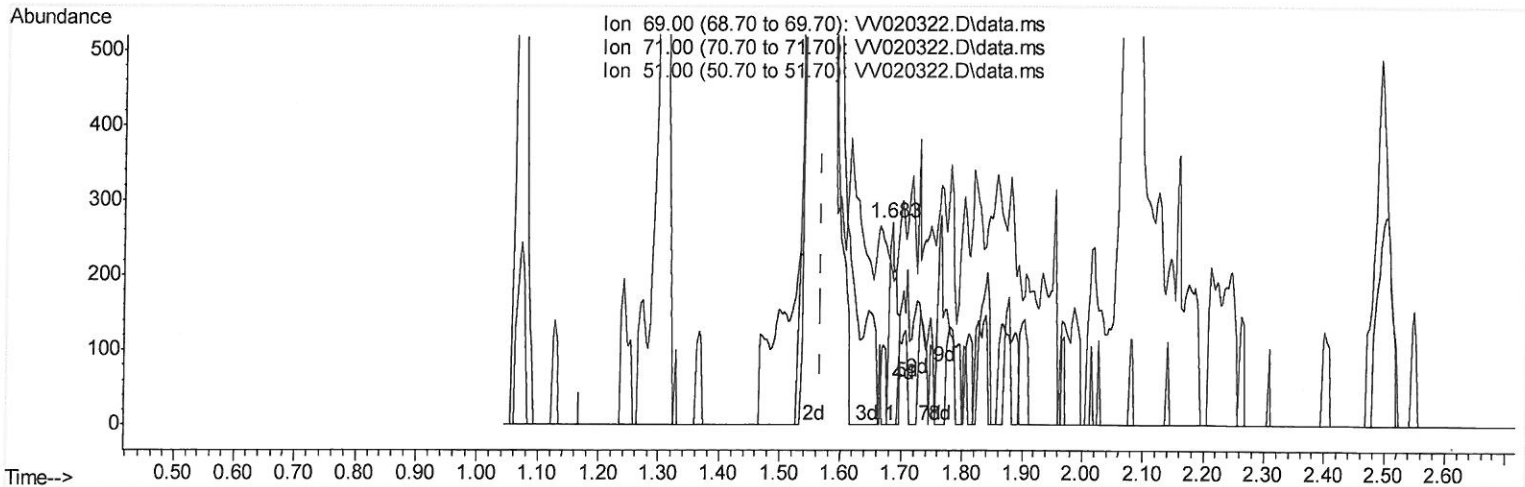

TIC: VW020322.D\data.ms

(7) Chloroethane-d5 (S)

1.683min (+ 0.116) 0.06 ug/L

response 233

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.30	25.75
51.00	26.90	33.91
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021521\
Data File : VV020322.D
Acq On : 15 Feb 2021 12:40
Operator : SY/MD
Sample : M1370-12ME
Misc : 4.75g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBGY8ME

Manual Integrations
APPROVED

MMDadoda
2/17/2021 10:34:59 AM

Quant Time: Feb 16 00:33:25 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Feb 16 00:32:19 2021
Response via : Initial Calibration

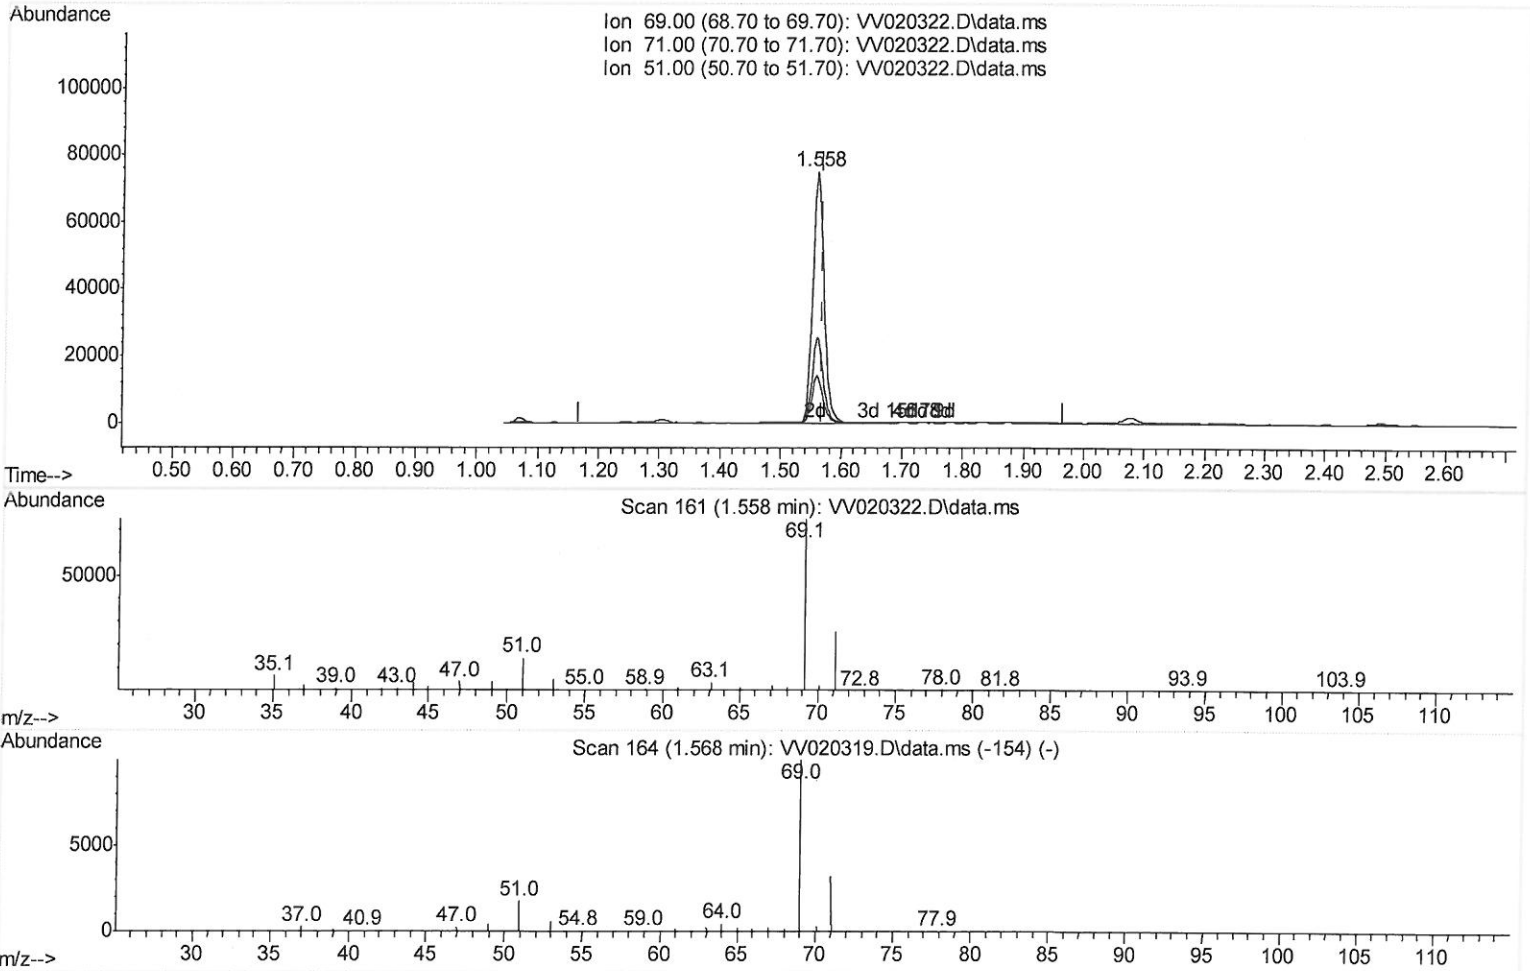

TIC: VV020322.D\data.ms

(7) Chloroethane-d5 (S)

1.558min (-0.010) 26.58 ug/L m

202/19/21 SY

response 96834

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.30	0.06#
51.00	26.90	0.08#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021521\
 Data File : VW020322.D
 Acq On : 15 Feb 2021 12:40
 Operator : SY/MD
 Sample : M1370-12ME
 Misc : 4.75g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleID :
 DBGY8ME

Manual Integrations
 APPROVED

MMDadoda
 2/17/2021 10:34:59 AM

Quant Time: Feb 16 00:33:25 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Feb 16 00:32:19 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	608932	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	593123	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.259	152	306159	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	163937	36.93	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 73.86%			
7) Chloroethane-d5	1.558	69	96834m	26.58	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 53.16%#			
11) 1,1-Dichloroethene-d2	2.076	63	253398	30.19	ug/L	-0.04
Spiked Amount 50.000	Range 60 - 125		Recovery = 60.38%			
21) 2-Butanone-d5	3.896	46	272744	109.96	ug/L	0.01
Spiked Amount 100.000	Range 40 - 130		Recovery = 109.96%			
24) Chloroform-d	4.343	84	331745	41.99	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 83.98%			
26) 1,2-Dichloroethane-d4	5.031	65	237430	47.40	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 94.80%			
32) Benzene-d6	5.040	84	688261	44.79	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 89.58%			
36) 1,2-Dichloropropane-d6	6.069	67	218930	47.72	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 95.44%			
41) Toluene-d8	7.317	98	636426	44.07	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 88.14%			
43) trans-1,3-Dichloroprop...	7.625	79	95029	40.64	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 81.28%			
47) 2-Hexanone-d5	8.127	63	213259	111.74	ug/L	0.04
Spiked Amount 100.000	Range 45 - 130		Recovery = 111.74%			
57) 1,1,2,2-Tetrachloroeth...	10.230	84	301421	45.76	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 91.52%			
64) 1,2-Dichlorobenzene-d4	11.635	152	267691	46.21	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 92.42%			
Target Compounds						
13) Acetone	2.182	43	134702	76.93	ug/L	96
42) Toluene	7.394	91	34953	2.00	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

2/19/21 SY

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\V021521\
Data File : V020322.D
Acq On : 15 Feb 2021 12:40
Operator : SY/MD
Sample : M1370-12ME
Misc : 4.75g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBGY8ME

Manual Integrations
APPROVED

MMDadoda
2/17/2021 10:34:59 AM

Quant Time: Feb 16 00:33:25 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Feb 16 00:32:19 2021
Response via : Initial Calibration

