
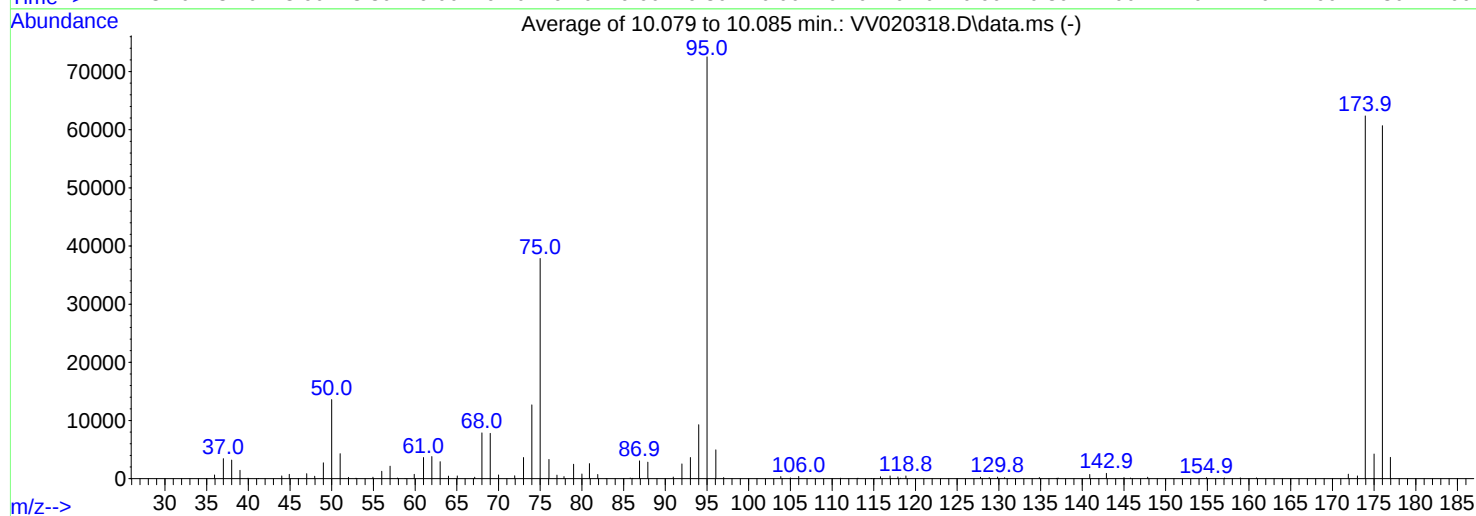


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021521\
 Data File : VV020318.D
 Acq On : 15 Feb 2021 09:10
 Operator : SY/MD
 Sample : BFB91
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB91

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
 Title : VOC Analysis
 Last Update : Tue Feb 16 00:32:19 2021

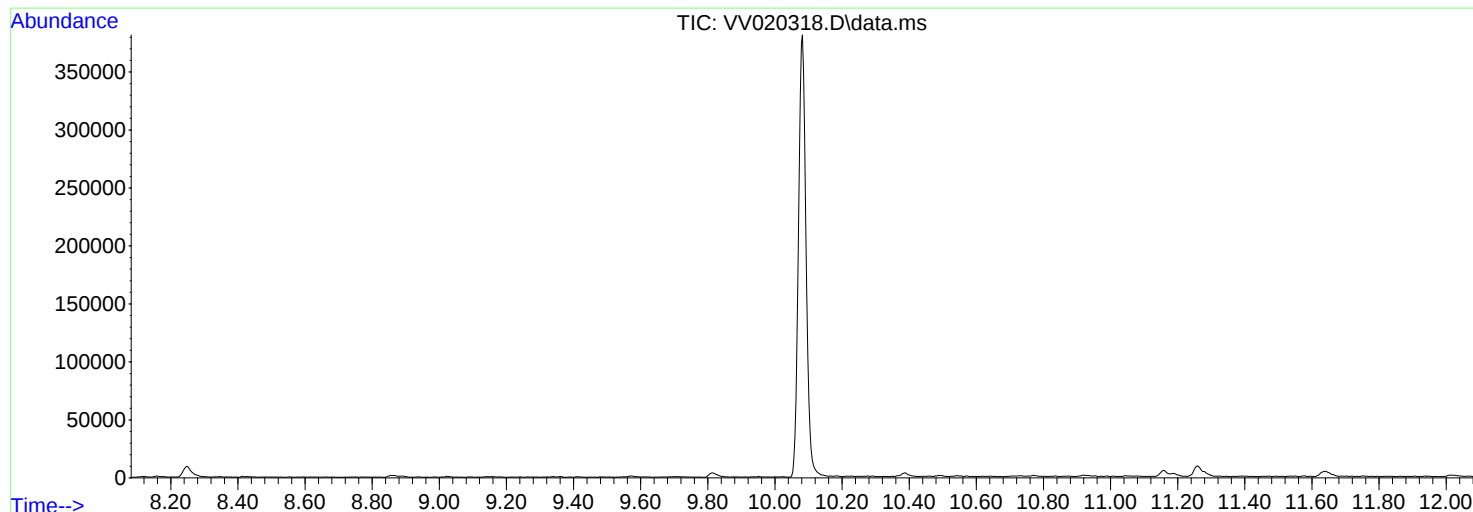

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	13581	PASS
75	95	30	80	52.2	37861	PASS
95	95	100	100	100.0	72528	PASS
96	95	5	9	6.8	4964	PASS
173	174	0.00	2	0.7	456	PASS
174	95	50	120	86.0	62376	PASS
175	174	5	9	6.8	4240	PASS
176	174	95	101	97.3	60699	PASS
177	176	5	9	6.0	3655	PASS

m/z	Abundance
36.00	618.0
37.00	3524.0
38.00	3264.0
39.00	1382.0
39.90	290.0
41.20	125.0
44.00	893.0
44.90	722.0
47.00	911.0
47.90	408.0
49.00	2918.0
50.00	14273.0
51.00	4463.0
52.00	240.0
52.90	143.0
54.90	319.0
56.00	1170.0
57.00	2253.0
57.90	141.0
58.80	109.0
59.90	710.0
61.00	3695.0
62.00	3949.0
63.00	2922.0
64.00	440.0
65.00	464.0
67.20	279.0
68.00	8031.0
69.00	8329.0
70.00	588.0
71.90	466.0
73.00	3760.0
74.00	13097.0
75.00	38544.0
76.00	3356.0
77.00	614.0
77.80	485.0
79.00	2576.0
80.00	825.0
80.90	2694.0
81.90	753.0
85.80	172.0
86.90	3135.0
87.90	3000.0
91.00	274.0
92.00	2576.0
93.00	3891.0
94.00	9663.0
95.00	74088.0
96.00	5292.0
97.00	165.0
103.90	297.0
105.00	145.0
106.00	363.0
111.00	106.0
114.70	108.0
115.80	349.0
116.90	512.0
118.00	344.0
118.90	458.0
127.80	283.0
128.80	198.0
129.90	255.0
130.70	159.0
134.80	170.0
136.90	134.0
140.90	707.0
142.00	121.0
142.90	863.0
145.10	175.0
145.80	126.0
147.80	224.0
155.00	192.0
157.10	102.0
159.00	118.0
160.90	140.0
171.90	763.0
173.00	672.0
174.00	61784.0
175.00	4366.0
176.00	59752.0
176.90	3762.0

Instrument :
MSVOA_V
ClientSampleId :
BFB91

m/z	Abundance
35.90	652.0
37.00	3551.0
38.00	3296.0
39.00	1432.0
39.90	286.0
40.90	128.0
44.00	940.0
44.90	768.0
47.00	890.0
47.90	409.0
49.00	2750.0
50.00	13922.0
51.00	4371.0
52.00	233.0
52.90	104.0
55.00	255.0
56.00	1327.0
57.00	2194.0
57.90	128.0
59.90	776.0
61.00	3757.0
62.00	3899.0
63.00	2998.0
64.00	469.0
65.00	462.0
67.10	261.0
68.00	8174.0
69.00	8011.0
70.00	622.0
71.90	509.0
73.00	3739.0
74.00	13046.0
75.00	39208.0
76.10	3459.0
77.00	638.0
77.90	361.0
79.00	2528.0
80.00	811.0
80.90	2660.0
81.90	756.0
85.80	173.0
86.90	3156.0
87.90	2891.0
90.90	278.0
92.00	2621.0
93.00	3770.0
94.00	9625.0
95.00	74880.0
96.00	5212.0
97.00	190.0
103.80	362.0
105.00	135.0
106.00	403.0
111.00	113.0
113.10	117.0
115.10	106.0
115.80	338.0
116.90	477.0
117.90	285.0
118.20	288.0
118.90	471.0
127.80	259.0
128.80	191.0
129.80	270.0
130.70	173.0
134.90	214.0
137.10	143.0
140.90	759.0
142.90	965.0
145.00	186.0
145.80	121.0
147.80	254.0
154.90	193.0
157.10	133.0
159.00	145.0
160.90	135.0
171.90	821.0
173.00	695.0
174.00	64528.0
175.00	4335.0
176.00	62960.0
176.90	3737.0

Instrument :
MSVOA_V
ClientSampleId :
BFB91

m/z	Abundance
35.00	650.0
37.00	3213.0
38.00	3062.0
39.00	1448.0
40.00	278.0
40.90	156.0
44.00	935.0
44.90	707.0
46.00	113.0
47.00	771.0
48.00	382.0
49.00	2498.0
50.00	12549.0
51.00	4030.0
52.00	201.0
54.90	181.0
56.00	1313.0
57.00	1974.0
57.90	109.0
59.90	721.0
61.00	3411.0
62.00	3545.0
63.00	2836.0
64.00	412.0
65.10	445.0
67.10	247.0
68.00	7392.0
69.00	7003.0
70.00	656.0
72.00	482.0
73.00	3391.0
74.00	11878.0
75.00	35832.0
76.00	3120.0
77.00	539.0
77.80	241.0
79.00	2327.0
80.00	738.0
80.90	2412.0
81.90	660.0
82.90	110.0
86.10	150.0
86.90	2916.0
87.90	2647.0
90.90	245.0
92.00	2403.0
93.00	3235.0
94.00	8516.0
95.00	68616.0
96.10	4387.0
97.00	199.0
103.80	420.0
105.00	123.0
106.00	369.0
113.10	138.0
115.80	285.0
117.00	428.0
117.80	279.0
118.80	490.0
127.80	224.0
128.90	162.0
129.80	290.0
130.70	162.0
134.90	203.0
137.10	188.0
140.90	727.0
142.90	939.0
144.90	182.0
145.80	104.0
147.90	231.0
154.80	176.0
157.00	127.0
158.90	148.0
160.90	113.0
171.90	774.0
173.90	60816.0
175.00	4020.0
176.00	59384.0
177.00	3467.0

Instrument :
MSVOA_V
ClientSampleId :
BFB91

m/z	Abundance
40.00	199.0
41.00	103.0
44.00	454.0

Instrument :
MSVOA_V
ClientSampleId :
BFB91