
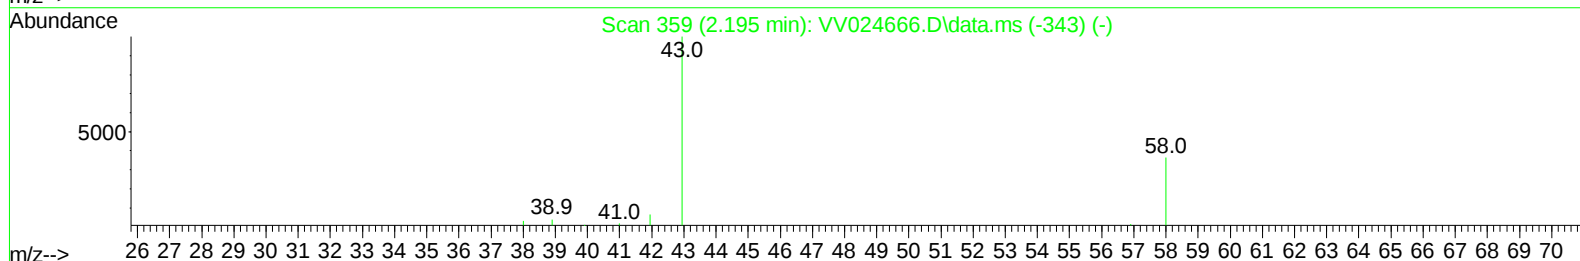
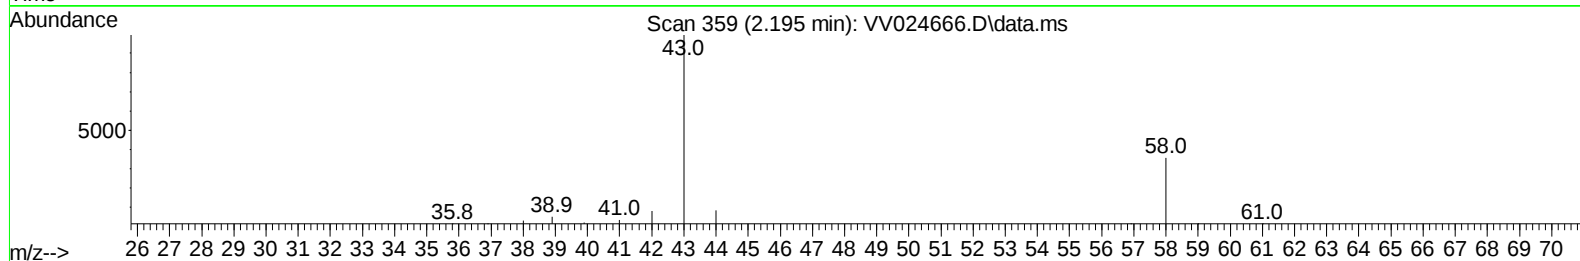


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021522\
Data File : VV024666.D
Acq On : 15 Feb 2022 12:36
Operator : SY/MD
Sample : VSTDCCC005
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Feb 16 03:26:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Feb 15 06:26:19 2022
Response via : Initial Calibration

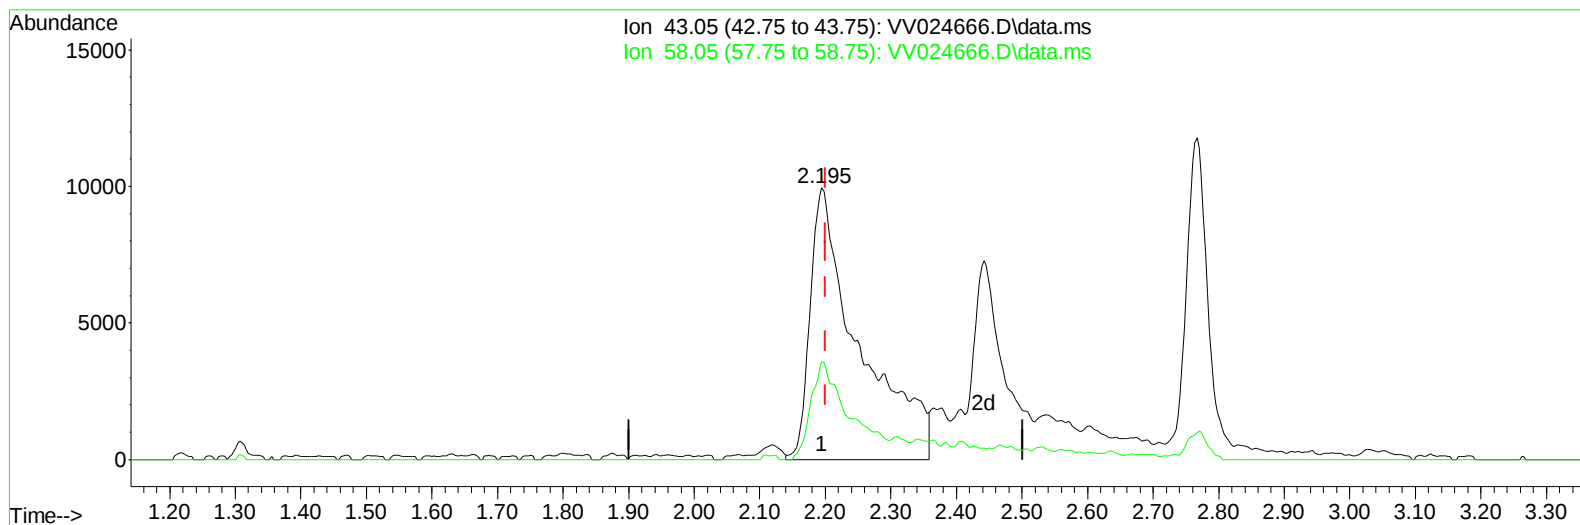

TIC: VV024666.D\data.ms

(13) Acetone (T)

2.195min (-0.007) 34.69 ug/L m

response 51344

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	28.55
0.00	0.00	0.00
0.00	0.00	0.00