

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021523\
 Data File : VV030052.D
 Acq On : 15 Feb 2023 14:18
 Operator : SY/MD
 Sample : VV0215WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK208

Quant Time: Feb 16 01:57:53 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM021523.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Feb 16 01:49:02 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	16640	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	14941	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	10537	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	5715	0.340	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	68.000%
4) 1,2-Dichloroethane-d4	4.946	65	4613	0.508	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	102.000%
7) 1,2-Dichloropropane-d6	5.995	67	5556	0.497	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	100.000%
8) Toluene-d8	7.253	98	17413	0.506	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	102.000%
10) 1,1,2,2-Tetrachloroeth...	10.146	84	4189	0.509	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	102.000%
Target Compounds						
6) Trichloroethene	5.852	95	216	0.018	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021523\
Data File : VV030052.D
Acq On : 15 Feb 2023 14:18
Operator : SY/MD
Sample : VV0215WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK208


Quant Time: Feb 16 01:57:53 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM021523.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Feb 16 01:49:02 2023
Response via : Initial Calibration

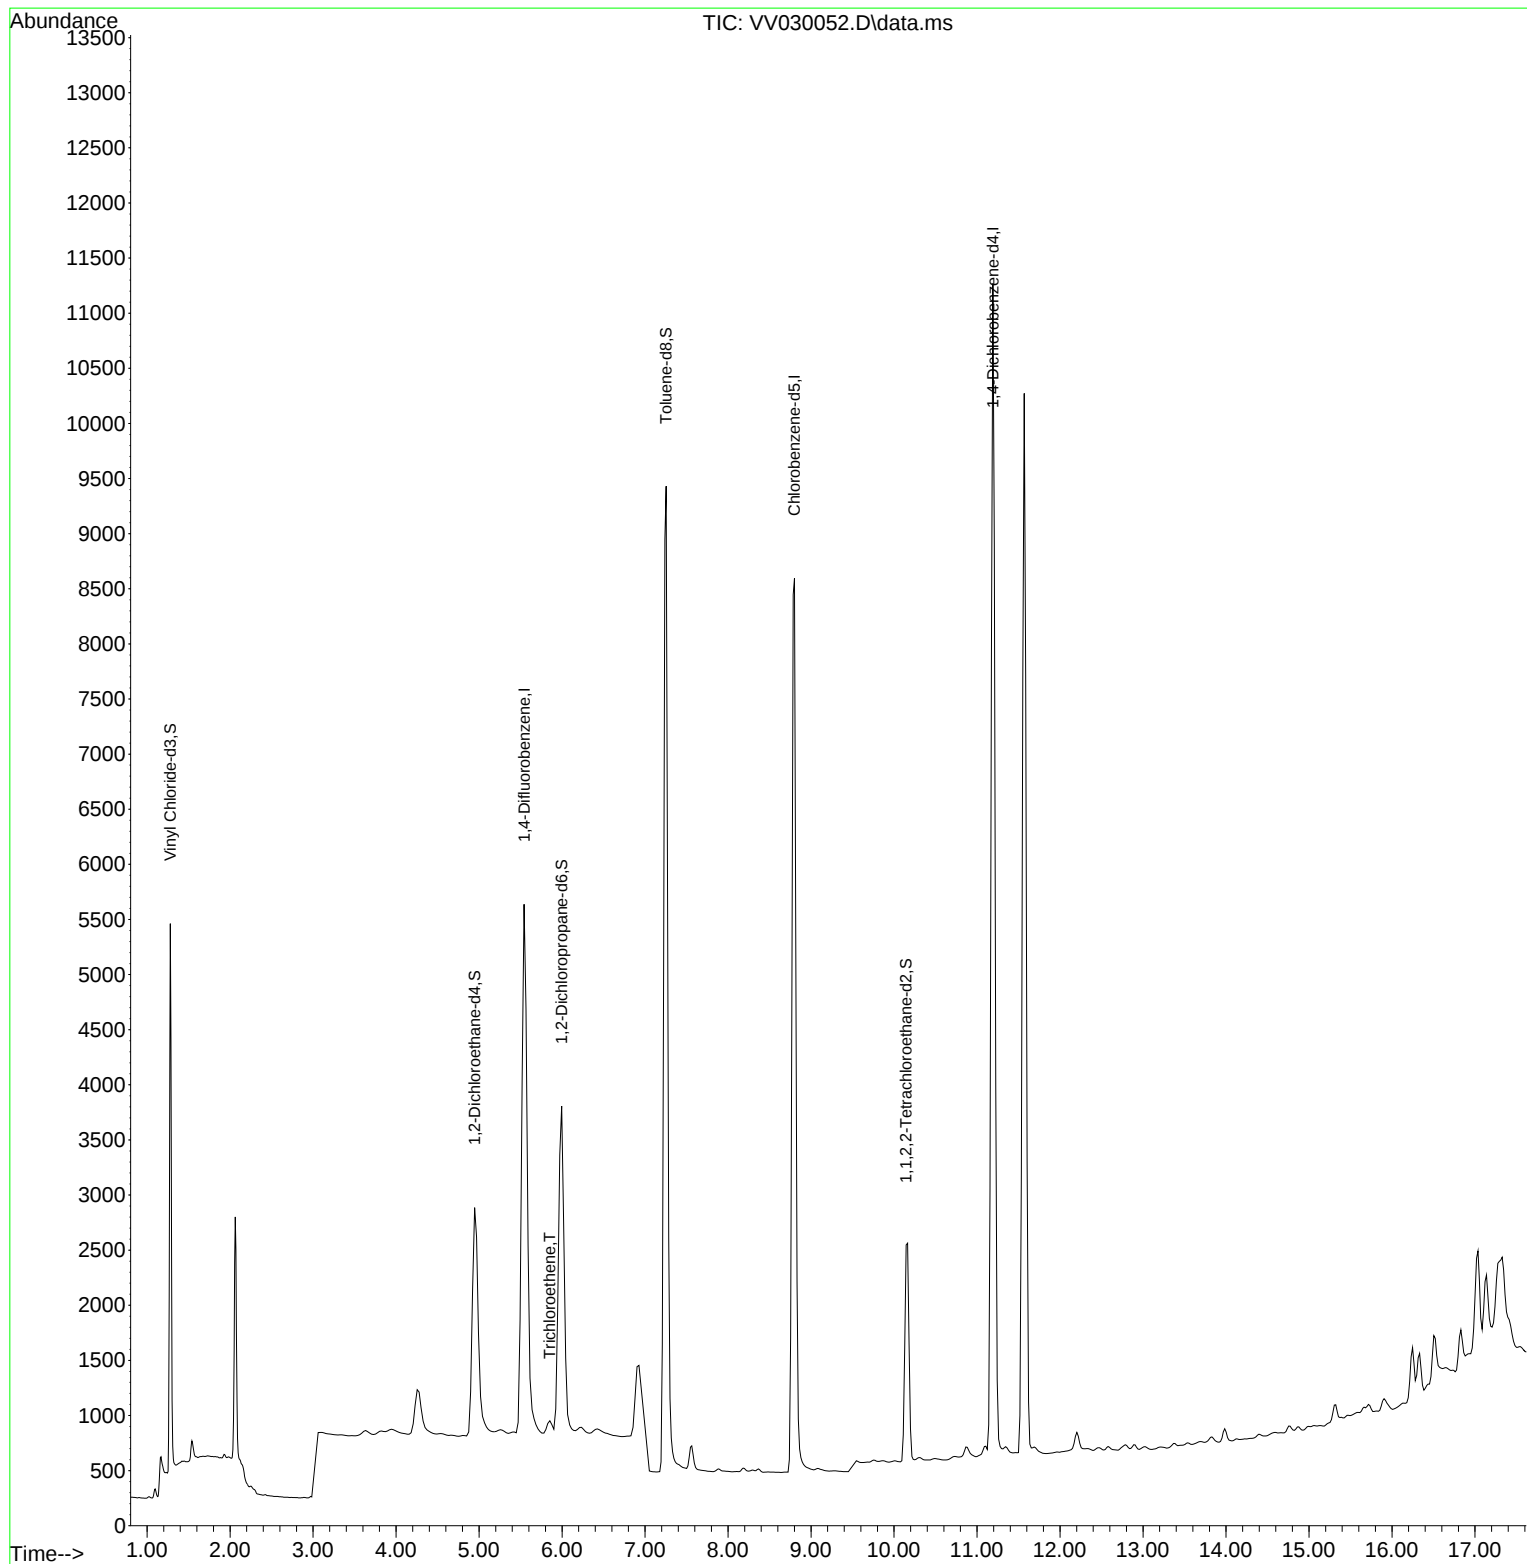

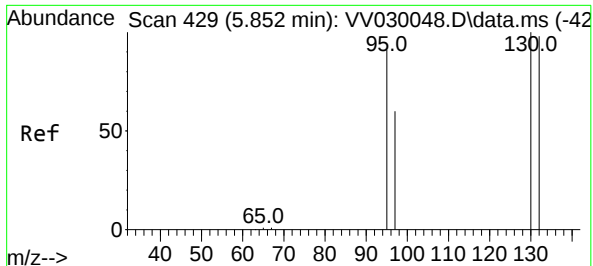

#6
 Trichloroethene
 Concen: 0.018 ug/L
 RT: 5.852 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: VV030052.D
 Acq: 15 Feb 2023 14:18

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK208

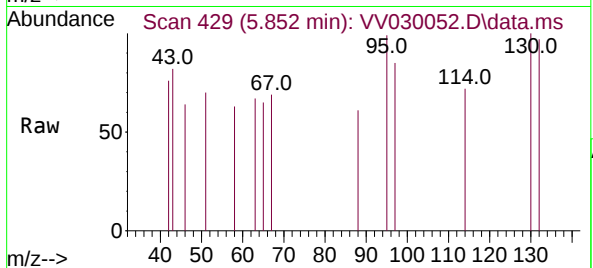

Tgt Ion: 95	Resp: 216
Ion Ratio	Lower Upper
95 100	
97 86.4	46.9 87.1
132 97.7	74.9 139.1
130 101.1	76.6 142.2

