




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021523\
 Data File : VV030046.D
 Acq On : 15 Feb 2023 11:41
 Operator : SY/MD
 Sample : VSTD0.0520
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.05220

Manual IntegrationsAPPROVED

Quant Time: Feb 16 01:31:21 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM021523.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Feb 16 01:30:38 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 02/16/2023
 Supervised By :Mahesh Dadoda 02/16/2023

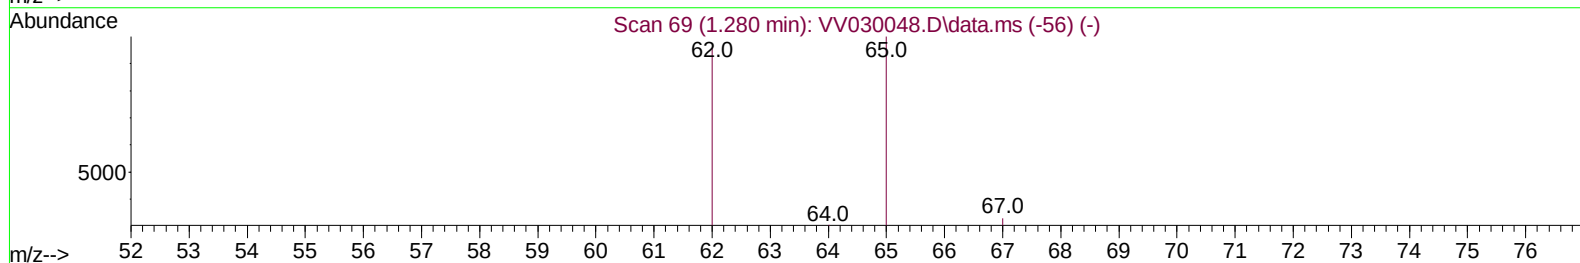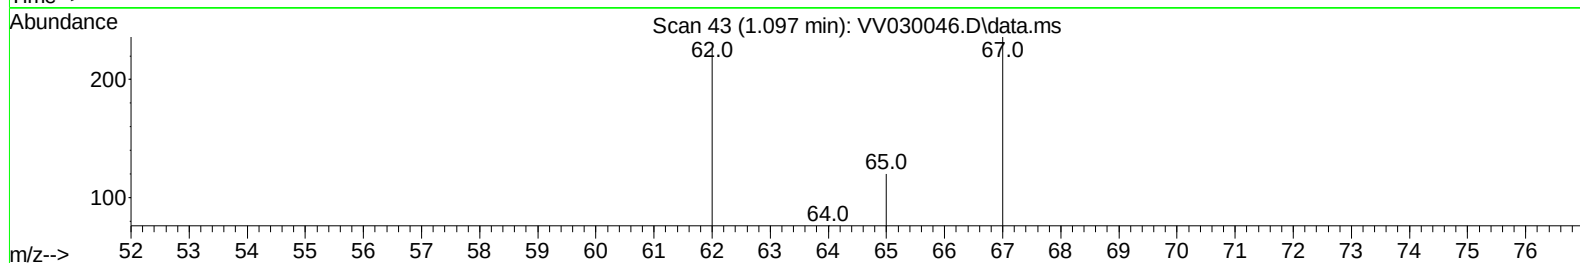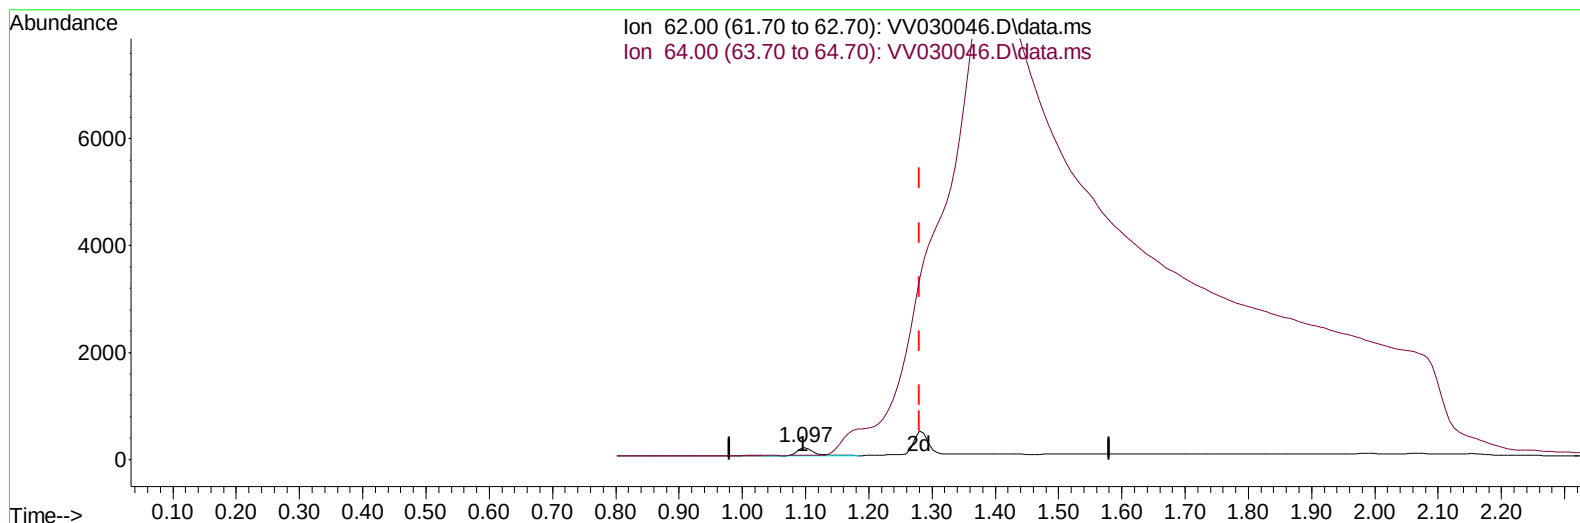

TIC: VV030046.D\data.ms

(3) Vinyl chloride (T)

1.097min (-0.183) 0.02 ug/L

response 313

Ion	Exp%	Act%
62.00	100.00	100.00
64.00	38.00	33.63
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021523\
 Data File : VV030046.D
 Acq On : 15 Feb 2023 11:41
 Operator : SY/MD
 Sample : VSTD0.0520
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.05220

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 02/16/2023
 Supervised By :Mahesh Dadoda 02/16/2023

Quant Time: Feb 16 01:31:21 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM021523.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Feb 16 01:30:38 2023
 Response via : Initial Calibration

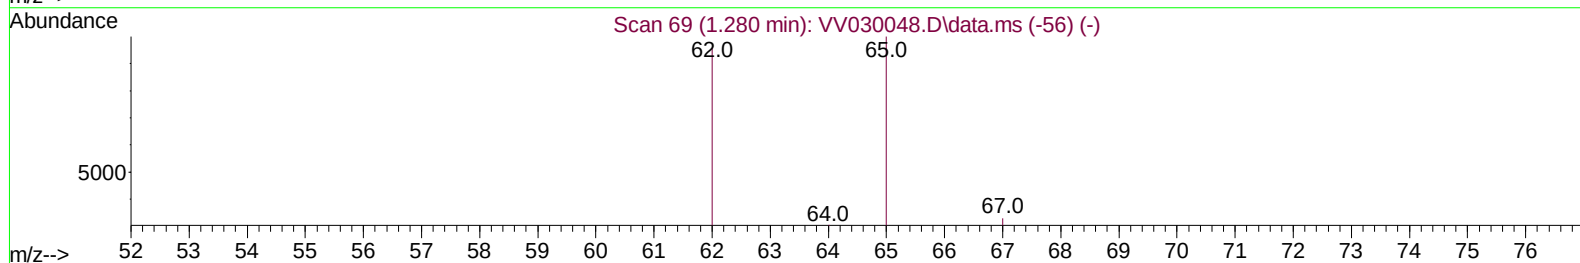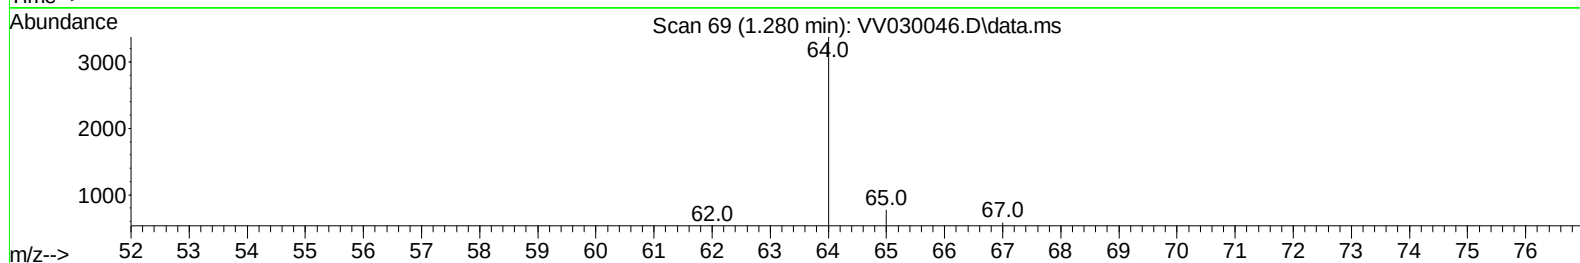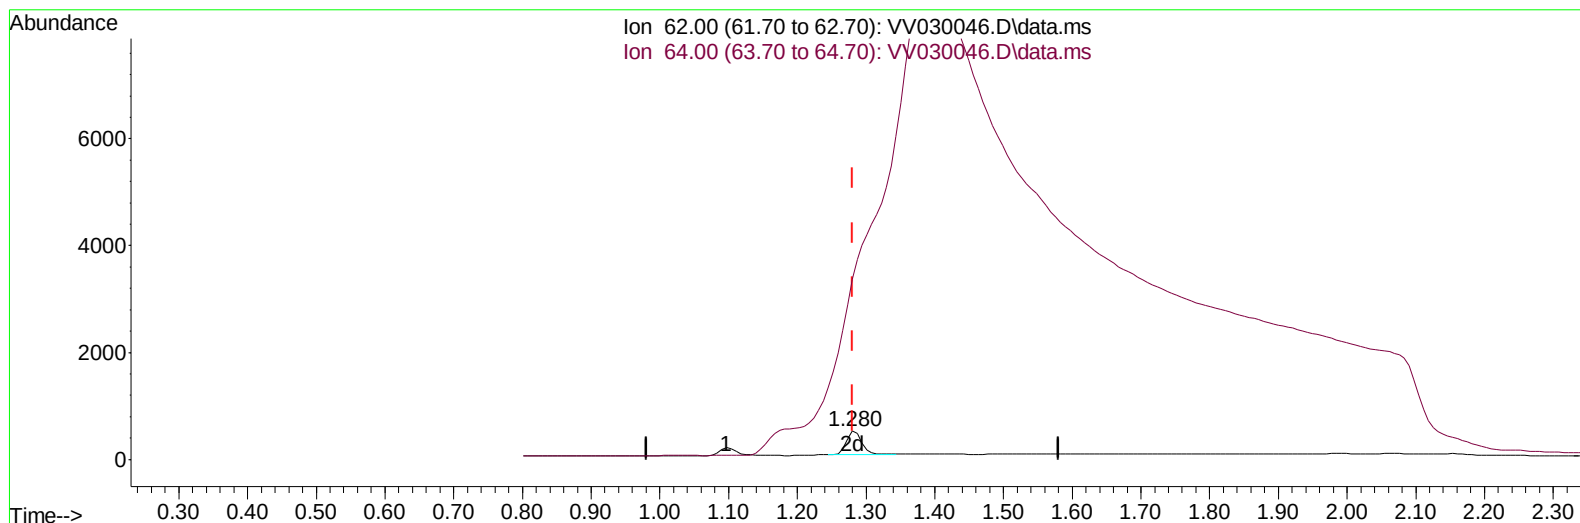

TIC: VV030046.D\data.ms

(3) Vinyl chloride (T)

1.280min (-0.000) 0.04 ug/L m

response 718

Ion	Exp%	Act%
62.00	100.00	100.00
64.00	38.00	630.65#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021523\
 Data File : VV030046.D
 Acq On : 15 Feb 2023 11:41
 Operator : SY/MD
 Sample : VSTD0.0520
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.05220

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 02/16/2023
 Supervised By :Mahesh Dadoda 02/16/2023

Quant Time: Feb 16 01:31:21 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM021523.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Feb 16 01:30:38 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.542	114		19691	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117		18586	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152		11264	0.500	ug/L	0.00
System Monitoring Compounds							
2) Vinyl Chloride-d3	1.280	65		1455	0.080	ug/L	0.00
4) 1,2-Dichloroethane-d4	4.945	65		538	0.048	ug/L	0.00
7) 1,2-Dichloropropane-d6	5.995	67		681	0.046	ug/L	0.00
8) Toluene-d8	7.253	98		2265	0.054	ug/L	0.00
10) 1,1,2,2-Tetrachloroeth...	10.146	84		518	0.053	ug/L	0.00
Target Compounds							Qvalue
3) Vinyl chloride	1.280	62		718m	0.042	ug/L	
6) Trichloroethene	5.828	95		800	0.057	ug/L	84
9) 1,2-Dibromoethane	8.290	107		380	0.046	ug/L #	94
12) 1,2,3-Trichloropropane	10.214	75		314	0.036	ug/L #	56
13) 1,2-Dibromo-3-chloropr...	12.356	75		104	0.065	ug/L	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021523\
Data File : VV030046.D
Acq On : 15 Feb 2023 11:41
Operator : SY/MD
Sample : VSTD0.0520
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.05220

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 02/16/2023
Supervised By :Mahesh Dadoda 02/16/2023

Quant Time: Feb 16 01:31:21 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM021523.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Feb 16 01:30:38 2023
Response via : Initial Calibration

