




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021523\
 Data File : VV030047.D
 Acq On : 15 Feb 2023 12:12
 Operator : SY/MD
 Sample : VSTD0.121
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.1221

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 02/16/2023
 Supervised By :Mahesh Dadoda 02/16/2023

Quant Time: Feb 16 01:31:32 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM021523.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Feb 16 01:30:38 2023
 Response via : Initial Calibration

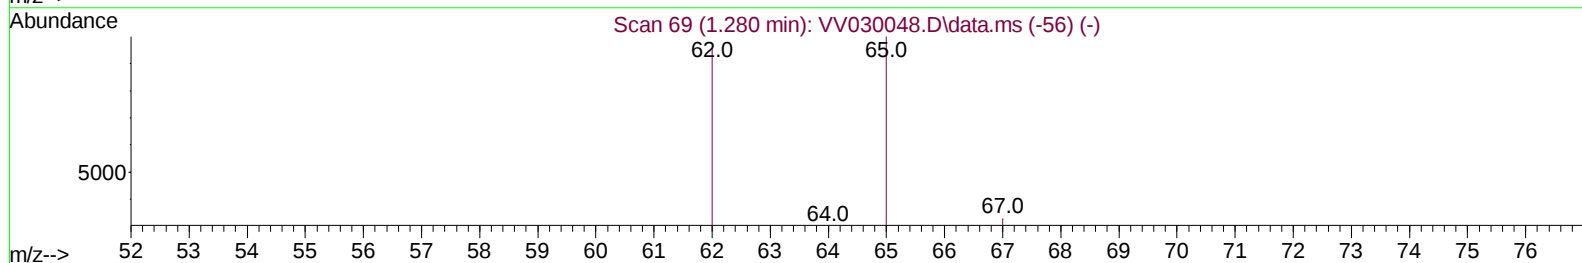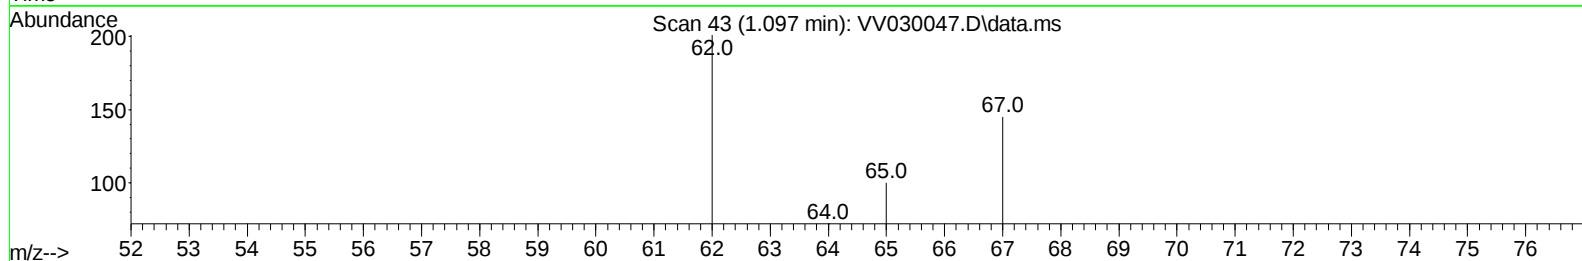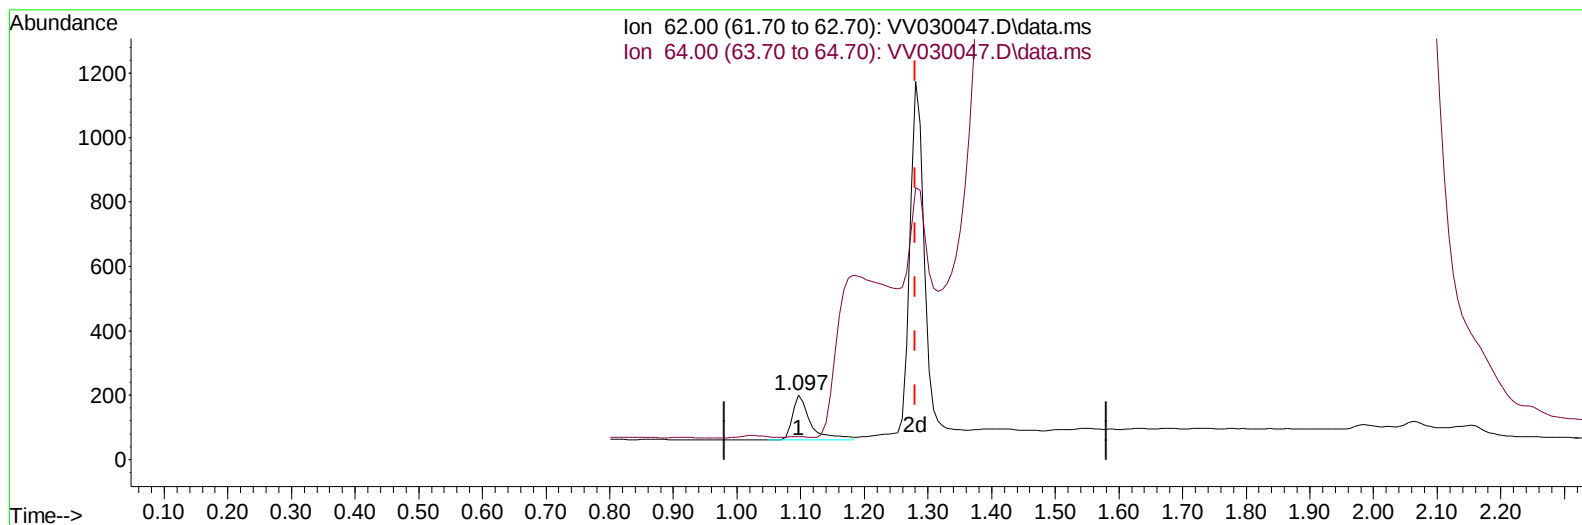

TIC: VV030047.D\data.ms

(3) Vinyl chloride (T)

1.097min (-0.183) 0.02 ug/L

response 276

Ion	Exp%	Act%
62.00	100.00	100.00
64.00	38.00	35.82
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021523\
 Data File : VV030047.D
 Acq On : 15 Feb 2023 12:12
 Operator : SY/MD
 Sample : VSTD0.121
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.1221

Manual IntegrationsAPPROVED

Quant Time: Feb 16 01:31:32 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM021523.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Feb 16 01:30:38 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 02/16/2023
 Supervised By :Mahesh Dadoda 02/16/2023

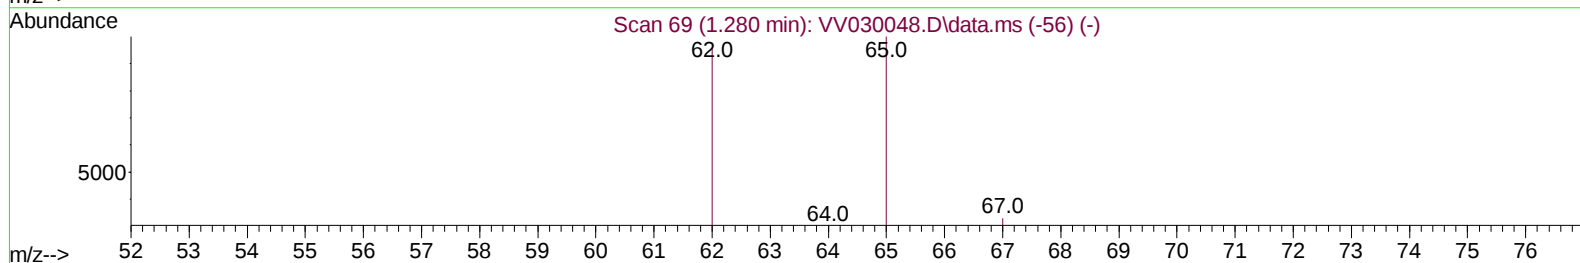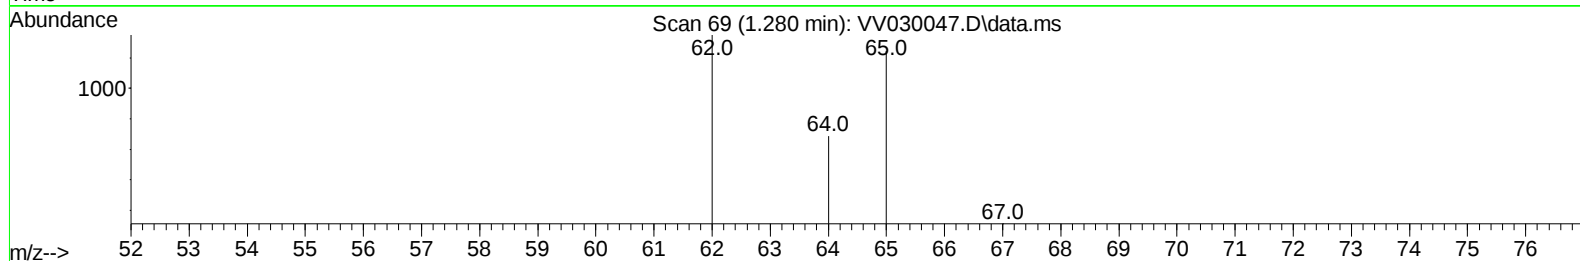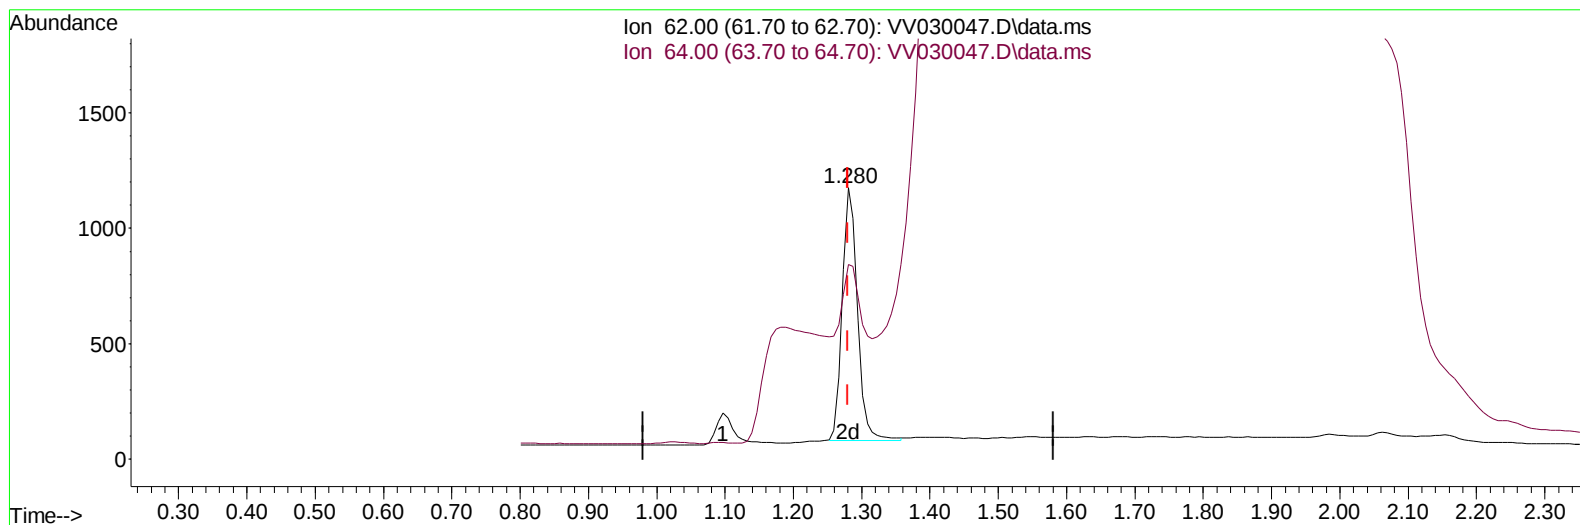

TIC: VV030047.D\data.ms

(3) Vinyl chloride (T)

1.280min (-0.000) 0.10 ug/L m

response 1697

Ion	Exp%	Act%
62.00	100.00	100.00
64.00	38.00	71.83#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021523\
 Data File : VV030047.D
 Acq On : 15 Feb 2023 12:12
 Operator : SY/MD
 Sample : VSTD0.121
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.1221

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 02/16/2023
 Supervised By :Mahesh Dadoda 02/16/2023

Quant Time: Feb 16 01:31:32 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM021523.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Feb 16 01:30:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	20286	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	19126	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	11192	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	1919	0.102	ug/L	0.00
4) 1,2-Dichloroethane-d4	4.946	65	948	0.082	ug/L	0.00
7) 1,2-Dichloropropane-d6	5.995	67	1247	0.082	ug/L	0.00
8) Toluene-d8	7.253	98	3880	0.089	ug/L	0.00
10) 1,1,2,2-Tetrachloroeth...	10.146	84	898	0.089	ug/L	0.00
Target Compounds						
						Qvalue
3) Vinyl chloride	1.280	62	1697m	0.095	ug/L	
6) Trichloroethene	5.852	95	1612	0.112	ug/L	97
9) 1,2-Dibromoethane	8.290	107	950	0.112	ug/L #	97
12) 1,2,3-Trichloropropane	10.214	75	820	0.096	ug/L #	89
13) 1,2-Dibromo-3-chloropr...	12.357	75	192	0.121	ug/L	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021523\
Data File : VV030047.D
Acq On : 15 Feb 2023 12:12
Operator : SY/MD
Sample : VSTD0.121
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.1221

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 02/16/2023
Supervised By :Mahesh Dadoda 02/16/2023

Quant Time: Feb 16 01:31:32 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM021523.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Feb 16 01:30:38 2023
Response via : Initial Calibration

