
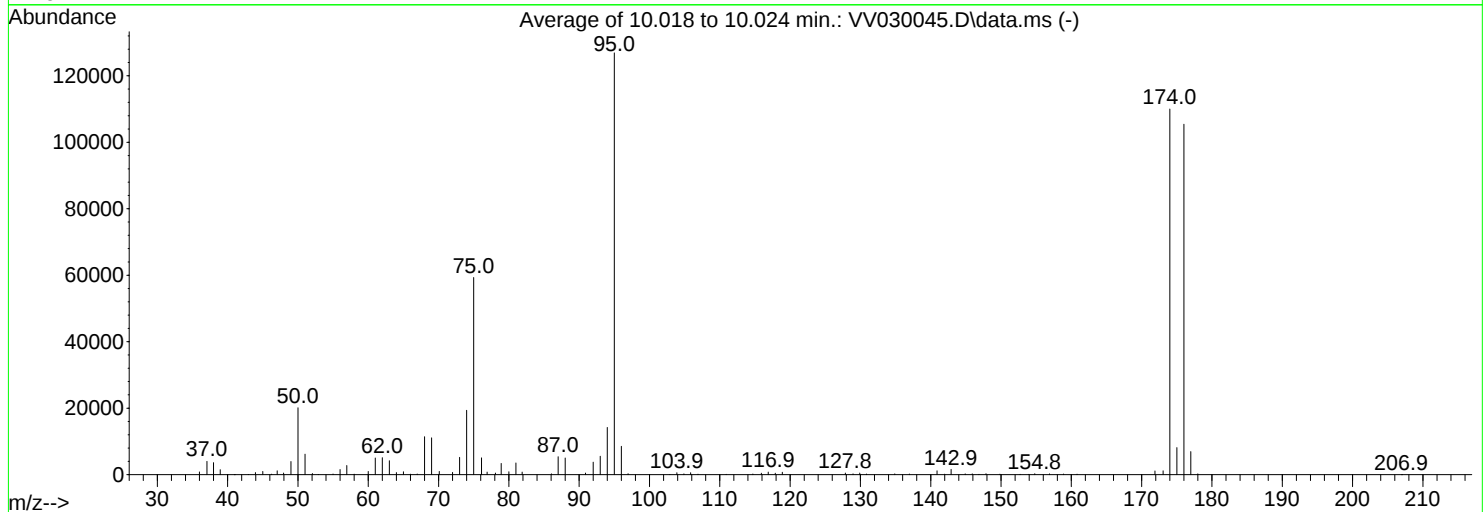


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021523\
Data File : VV030045.D
Acq On : 15 Feb 2023 10:39
Operator : SY/MD
Sample : BFB222
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB222

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM021523.M
Title : TRACE VOA SOM01.0
Last Update : Thu Feb 16 01:49:02 2023

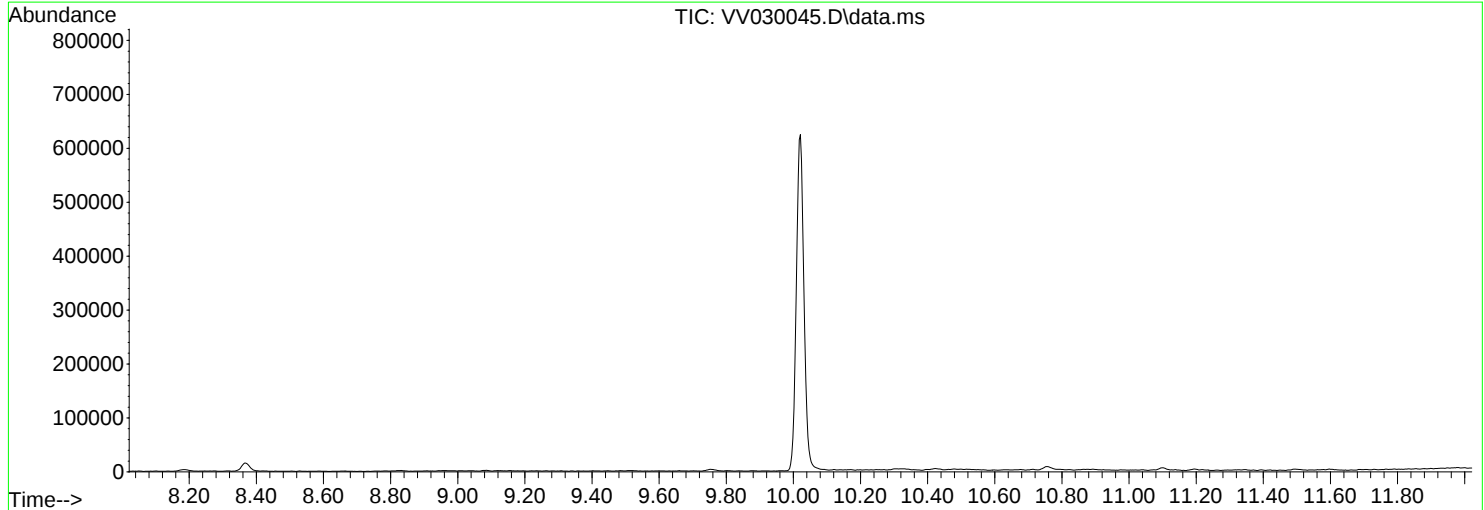

AutoFind: Scans 2792, 2793, 2794; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	20139	PASS
75	95	30	80	46.7	59323	PASS
95	95	100	100	100.0	126907	PASS
96	95	5	9	6.7	8513	PASS
173	174	0.00	2	1.1	1178	PASS
174	95	50	120	86.7	110000	PASS
175	174	5	9	7.4	8155	PASS
176	174	95	101	95.8	105435	PASS
177	176	5	9	6.6	6959	PASS

m/z	Abundance
38.90	104.0
40.00	162.0
41.00	132.0
43.00	192.0
43.90	743.0
55.00	210.0
56.90	152.0
66.90	119.0
207.00	148.0

Instrument :
MSVOA_V
ClientSampleId :
BFB222

m/z	Abundance
36.00	865.0
37.00	4278.0
38.00	3682.0
39.00	1608.0
40.00	236.0
41.00	184.0
42.90	201.0
44.00	1420.0
45.00	976.0
46.30	152.0
47.10	1230.0
48.00	551.0
49.00	4255.0
50.00	20720.0
51.00	6383.0
52.00	330.0
52.90	115.0
55.00	430.0
56.00	1593.0
57.00	3020.0
58.00	146.0
60.00	1014.0
61.00	5308.0
62.00	5264.0
63.00	4443.0
64.00	621.0
65.00	837.0
66.00	147.0
67.00	346.0
68.00	11663.0
69.00	11483.0
70.10	1070.0
72.00	711.0
73.00	5368.0
74.00	19960.0
75.00	61280.0
76.10	5117.0
76.90	810.0
78.10	463.0
78.90	3410.0
80.00	901.0
81.00	3639.0
81.90	791.0
86.10	199.0
87.00	5607.0
88.00	5129.0
90.90	511.0
92.00	3696.0
93.00	5783.0
94.00	14605.0
95.00	130120.0
96.00	8742.0
97.00	292.0
103.90	632.0
104.90	227.0
105.90	589.0
106.90	158.0
110.90	123.0
114.70	199.0
115.90	501.0
116.90	839.0
117.90	443.0
118.90	715.0
127.90	456.0
128.90	281.0
129.90	467.0
130.80	170.0
134.90	257.0
137.00	205.0
140.90	1156.0
142.00	188.0
142.90	1622.0
144.90	291.0
145.90	207.0
146.90	112.0
147.90	285.0
149.80	146.0
153.90	118.0
154.80	310.0
156.80	238.0
158.90	226.0
160.80	205.0
171.90	1082.0
173.00	1161.0
174.00	109864.0
175.00	8126.0
176.00	104936.0
177.00	7296.0
178.00	234.0
207.00	169.0

Instrument :
MSVOA_V
ClientSampleId :
BFB222

m/z	Abundance
36.00	854.0
37.10	4111.0
38.00	3768.0
39.00	1701.0
40.00	225.0
41.00	153.0
42.90	220.0
44.00	1429.0
45.00	988.0
46.20	151.0
47.10	1190.0
47.90	504.0
49.00	4038.0
50.00	20856.0
51.00	6338.0
52.00	369.0
52.90	101.0
55.00	448.0
56.00	1567.0
57.00	2986.0
58.00	163.0
60.00	1006.0
61.00	5156.0
62.00	5260.0
63.00	4326.0
64.00	637.0
65.00	891.0
66.00	138.0
67.00	336.0
68.00	11862.0
69.00	11368.0
70.10	962.0
72.00	725.0
73.00	5376.0
74.00	19992.0
75.00	61144.0
76.10	5201.0
76.90	808.0
78.10	521.0
78.90	3549.0
80.00	866.0
81.00	3640.0
81.90	784.0
86.00	280.0
87.00	5530.0
88.00	5187.0
90.90	507.0
92.00	3902.0
93.00	5703.0
94.00	14654.0
95.00	131200.0
96.00	8762.0
96.90	299.0
102.90	109.0
103.90	605.0
104.90	257.0
105.90	608.0
106.90	147.0
110.90	128.0
114.70	225.0
115.90	465.0
116.90	823.0
117.90	445.0
118.90	786.0
127.90	508.0
128.90	273.0
129.90	493.0
130.90	182.0
134.90	264.0
136.90	207.0
140.90	1171.0
142.00	183.0
142.90	1626.0
144.90	256.0
145.90	265.0
146.90	117.0
147.90	305.0
149.80	145.0
152.70	119.0
153.90	120.0
154.80	309.0
156.90	257.0
158.90	220.0
160.80	174.0
171.90	1142.0
173.00	1194.0
174.00	113512.0
175.00	8494.0
176.00	109080.0
177.00	7088.0
178.00	240.0
207.00	153.0

Instrument :
MSVOA_V
ClientSampleId :
BFB222

m/z	Abundance
36.00	744.0
37.10	3621.0
38.00	3439.0
39.00	1534.0
40.00	215.0
40.90	129.0
43.00	262.0
44.00	1328.0
45.00	890.0
46.20	147.0
47.00	1112.0
48.00	463.0
49.00	3549.0
50.00	18840.0
51.00	5818.0
52.10	357.0
55.00	419.0
56.00	1405.0
57.00	2703.0
58.00	144.0
60.00	906.0
61.00	4636.0
62.00	4822.0
63.00	3824.0
64.00	565.0
65.00	863.0
66.00	100.0
67.00	318.0
68.00	10773.0
69.00	10398.0
70.10	842.0
72.00	657.0
73.00	4932.0
74.00	18136.0
75.00	55544.0
76.10	4915.0
76.90	728.0
78.10	544.0
78.90	3232.0
80.00	825.0
81.00	3319.0
81.90	717.0
86.00	320.0
87.00	5021.0
88.00	4761.0
90.90	483.0
92.00	3750.0
93.00	5137.0
94.00	13329.0
95.00	119400.0
96.00	8034.0
97.00	338.0
102.90	109.0
103.90	542.0
104.90	254.0
105.80	520.0
106.90	128.0
110.90	112.0
114.70	218.0
115.90	382.0
116.90	736.0
117.90	409.0
118.90	724.0
127.80	510.0
129.00	254.0
129.90	452.0
130.90	176.0
134.90	246.0
136.90	201.0
140.90	1139.0
142.00	150.0
142.90	1482.0
144.90	211.0
145.90	243.0
146.80	106.0
147.80	293.0
149.90	135.0
152.70	130.0
154.00	109.0
154.80	294.0
157.00	264.0
158.90	158.0
160.80	143.0
171.90	1173.0
173.10	1180.0
174.00	106624.0
175.00	7846.0
176.00	102288.0
177.00	6494.0
178.00	197.0
206.90	141.0

Instrument :
MSVOA_V
ClientSampleId :
BFB222