




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021524\
 Data File : VV034186.D
 Acq On : 15 Feb 2024 13:55
 Operator : SY/MD
 Sample : P1498-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG1

Manual IntegrationsAPPROVED

Quant Time: Feb 16 00:41:47 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 16 00:40:49 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 02/16/2024
 Supervised By :Semsettin Yesilyurt 02/16/2024

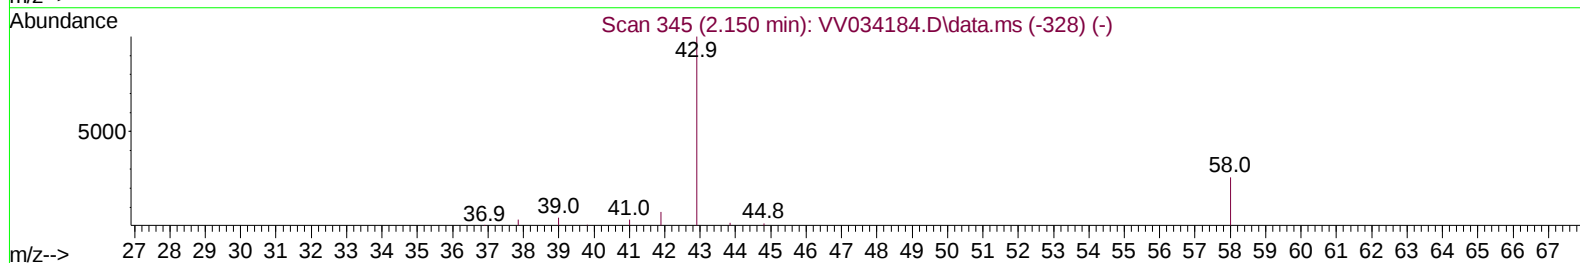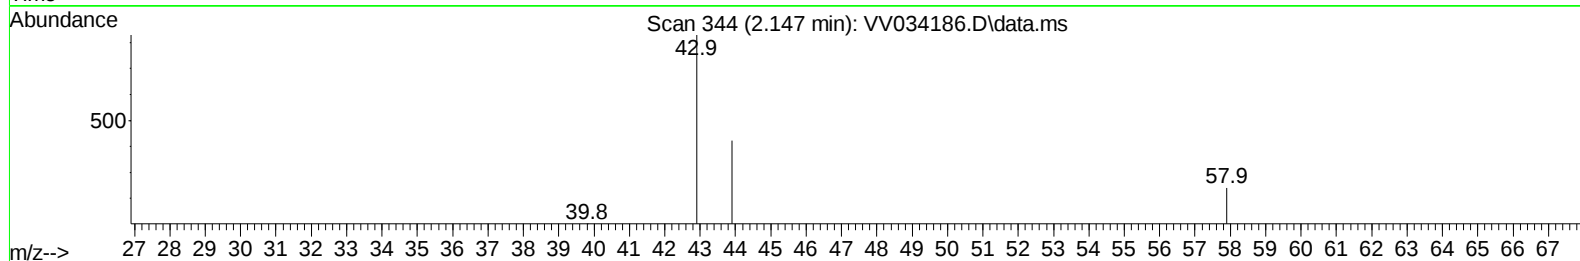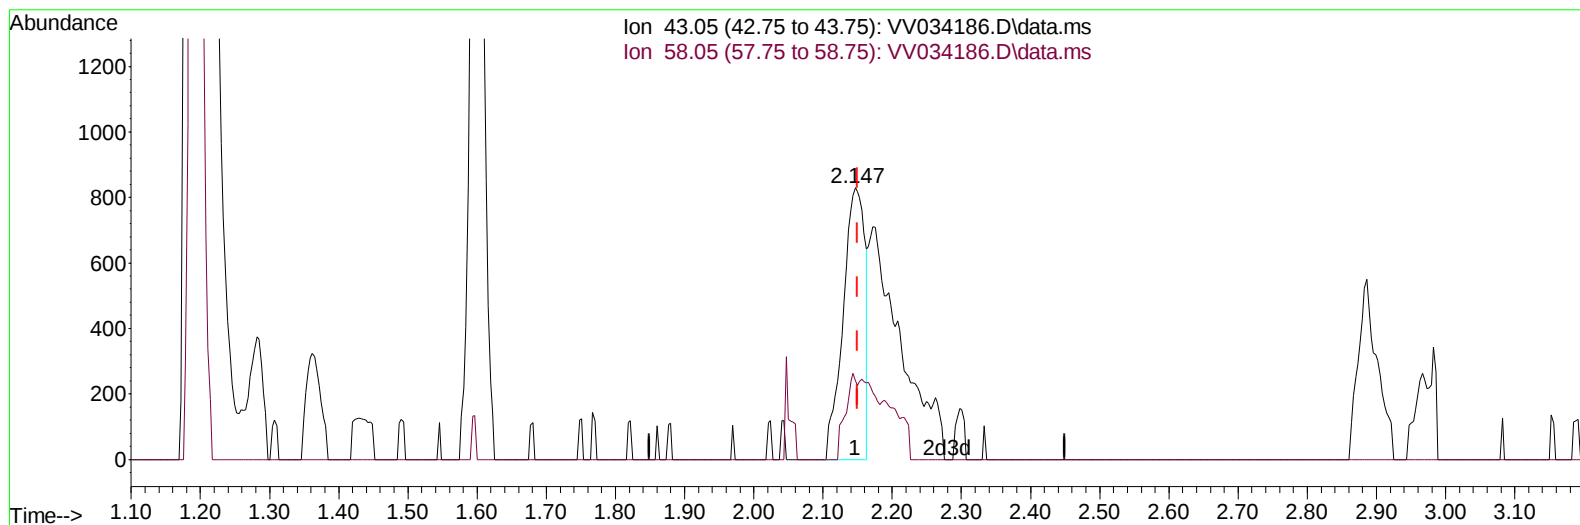

TIC: VV034186.D\data.ms

(13) Acetone (T)

2.147min (-0.003) 2.20 ug/L

response 1808

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	6.90	17.53#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021524\
Data File : VV034186.D
Acq On : 15 Feb 2024 13:55
Operator : SY/MD
Sample : P1498-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG1

Manual IntegrationsAPPROVED

Quant Time: Feb 16 00:41:47 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 16 00:40:49 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 02/16/2024
Supervised By :Semsettin Yesilyurt 02/16/2024

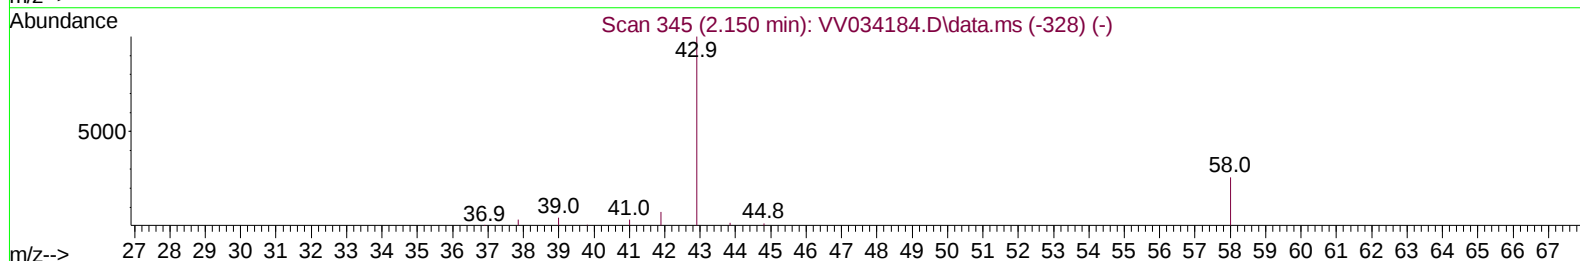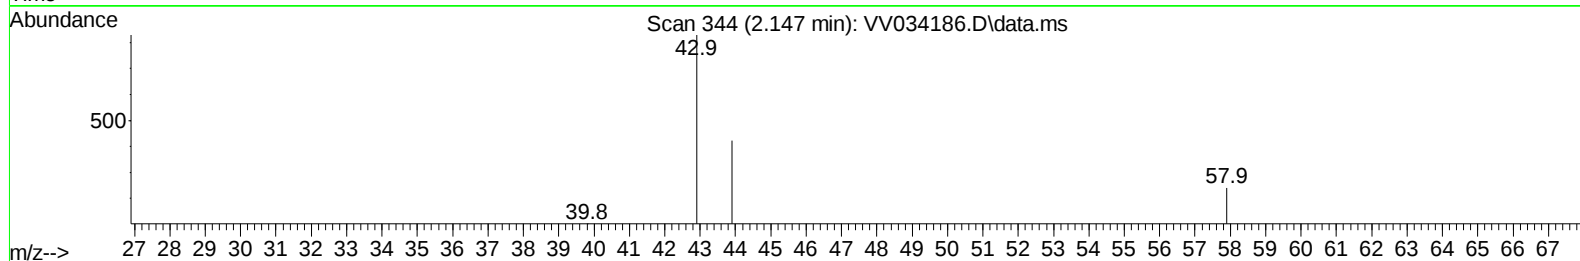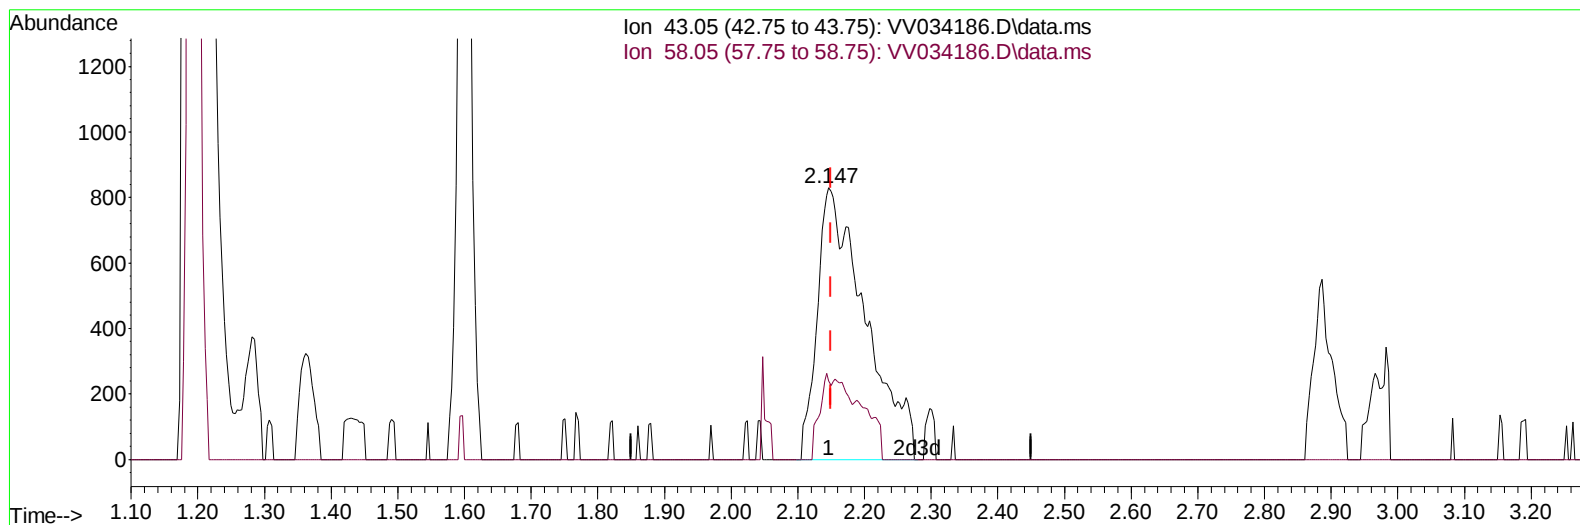

TIC: VV034186.D\data.ms

(13) Acetone (T)

2.147min (-0.003) 5.02 ug/L m

response 4127

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	6.90	7.68
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021524\
 Data File : VV034186.D
 Acq On : 15 Feb 2024 13:55
 Operator : SY/MD
 Sample : P1498-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG1

Manual IntegrationsAPPROVED

Quant Time: Feb 16 00:41:47 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 16 00:40:49 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 02/16/2024
 Supervised By :Semsettin Yesilyurt 02/16/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.532	114		83376	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117		75876	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152		38998	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.282	65		21381	3.311	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	66.200%	
7) Chloroethane-d5	1.536	69		21272	3.761	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	75.200%	
11) 1,1-Dichloroethene-d2	2.060	65		11107	3.567	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	71.400%	
20) 2-Butanone-d5	3.828	46		38726	35.709	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	71.420%	
24) Chloroform-d	4.249	84		49305	4.202	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	84.000%	
26) 1,2-Dichloroethane-d4	4.944	65		23972	4.372	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	87.400%	
32) Benzene-d6	4.960	84		89885	3.948	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	79.000%	
36) 1,2-Dichloropropane-d6	5.989	67		24830	3.902	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	78.000%	
41) Toluene-d8	7.243	98		82146	3.926	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	78.600%	
43) trans-1,3-Dichloroprop...	7.558	79		9224	3.839	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	76.800%	
46) 2-Hexanone-d5	8.027	63		28421	33.134	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	66.260%	
56) 1,1,2,2-Tetrachloroeth...	10.153	84		14645	3.796	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	76.000%	
66) 1,2-Dichlorobenzene-d4	11.561	152		29776	4.198	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	84.000%	
Target Compounds							
13) Acetone	2.147	43		4127m	5.016	ug/L	
16) Methylene chloride	2.449	84		1547	0.277	ug/L	98
42) Toluene	7.326	91		4894	0.201	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021524\
Data File : VV034186.D
Acq On : 15 Feb 2024 13:55
Operator : SY/MD
Sample : P1498-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG1

Manual IntegrationsAPPROVED

Quant Time: Feb 16 00:41:47 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 16 00:40:49 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 02/16/2024
Supervised By :Semsettin Yesilyurt 02/16/2024

