

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021524\
 Data File : VV034193.D
 Acq On : 15 Feb 2024 17:30
 Operator : SY/MD
 Sample : VIBLK323
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK323

Quant Time: Feb 16 00:43:45 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 16 00:40:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	74513	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	67324	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	31097	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	19487	3.377	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	67.600%
7) Chloroethane-d5	1.535	69	18795	3.718	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	74.400%
11) 1,1-Dichloroethene-d2	2.060	65	10528	3.783	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.600%
20) 2-Butanone-d5	3.834	46	43895	45.290	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	90.580%
24) Chloroform-d	4.252	84	46735	4.457	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.200%
26) 1,2-Dichloroethane-d4	4.947	65	24207	4.940	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.800%
32) Benzene-d6	4.963	84	82939	4.106	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.200%
36) 1,2-Dichloropropane-d6	5.989	67	24515	4.342	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	86.800%
41) Toluene-d8	7.243	98	76113	4.100	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.000%
43) trans-1,3-Dichloroprop...	7.561	79	9083	4.260	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.200%
46) 2-Hexanone-d5	8.030	63	36557	48.033	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.060%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	16316	4.767	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.400%
66) 1,2-Dichlorobenzene-d4	11.561	152	27019	4.777	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.600%
Target Compounds						Qvalue
34) Trichloroethene	5.838	95	8325	1.425	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021524\
Data File : VV034193.D
Acq On : 15 Feb 2024 17:30
Operator : SY/MD
Sample : VIBLK323
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK323


Quant Time: Feb 16 00:43:45 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 16 00:40:49 2024
Response via : Initial Calibration

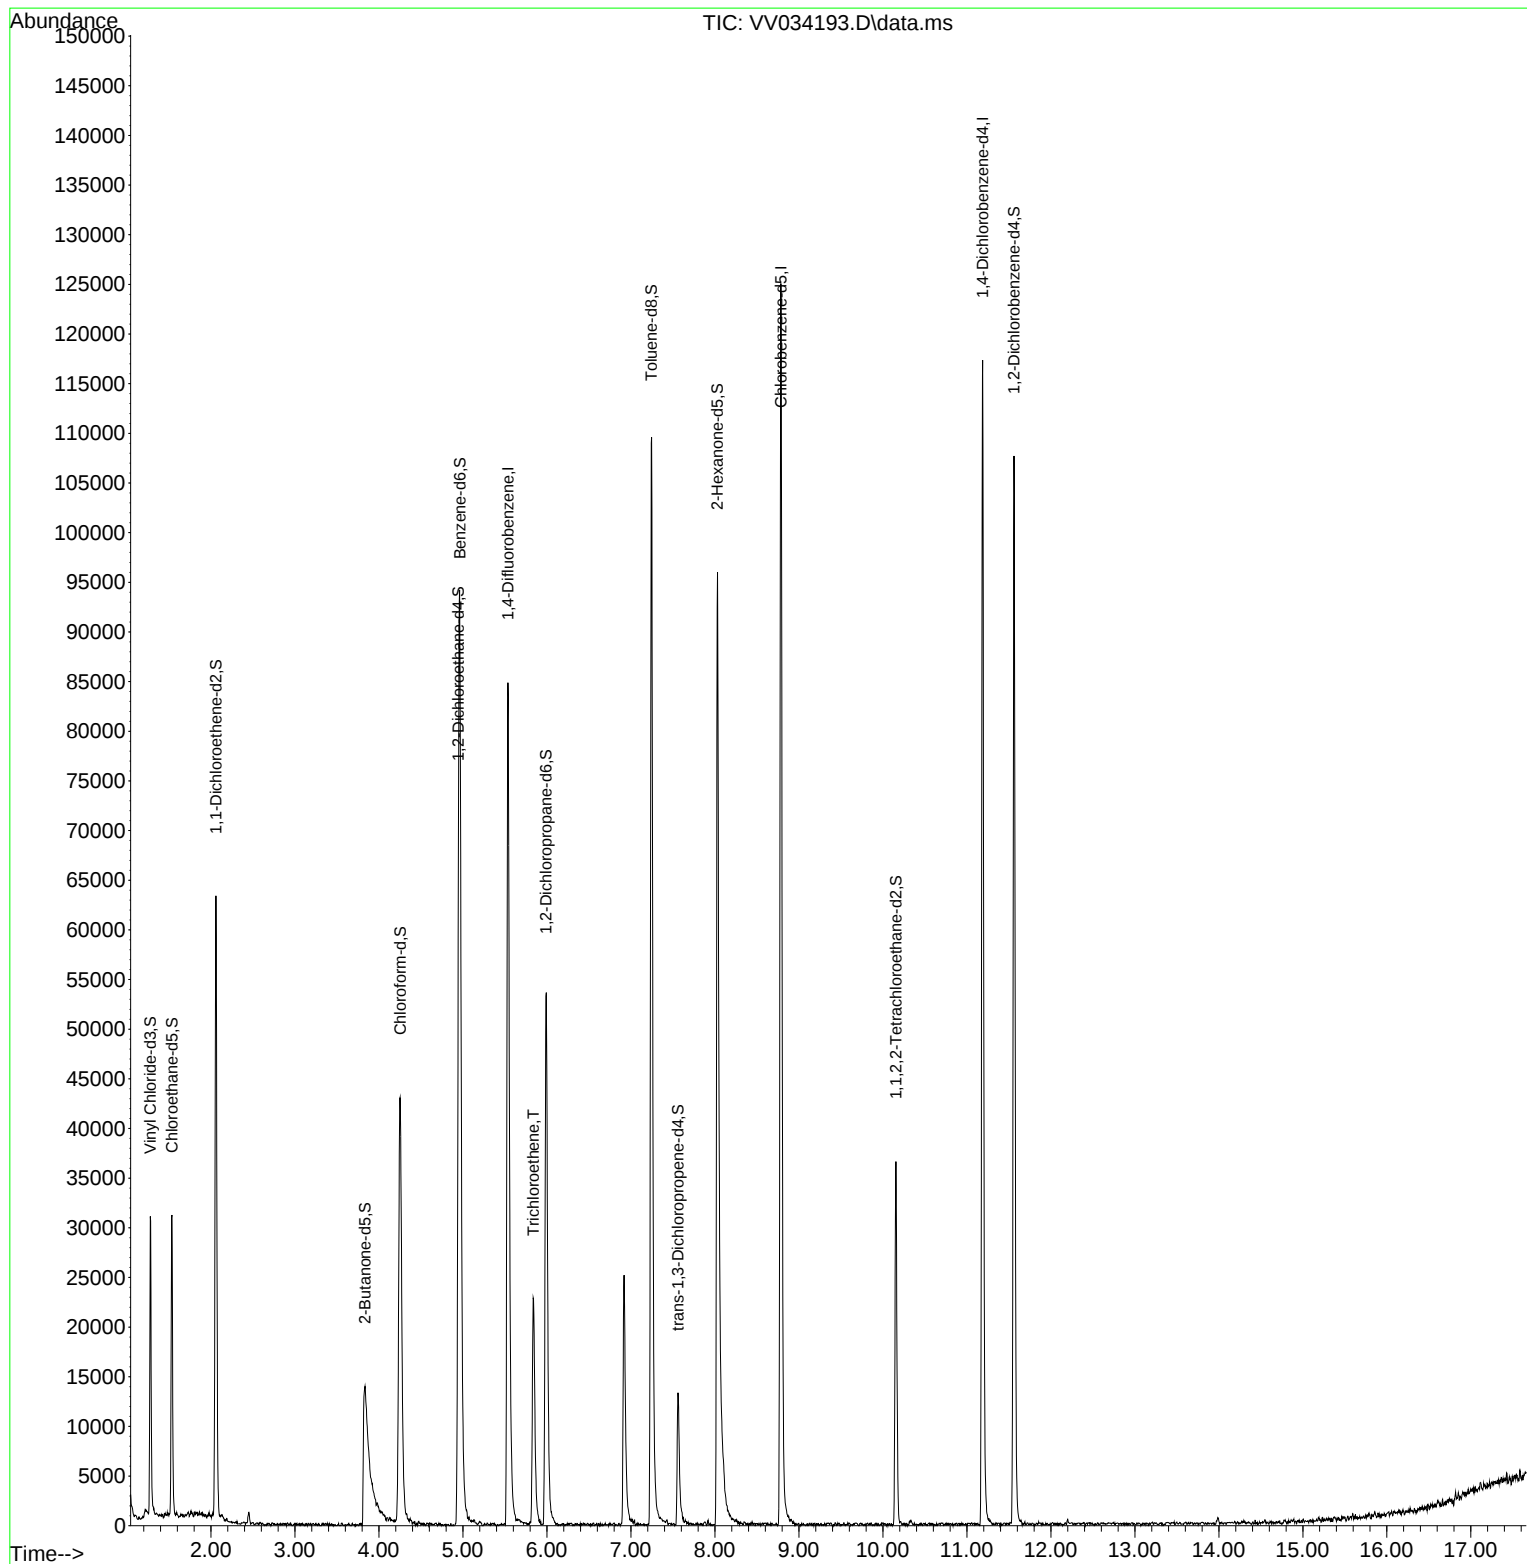

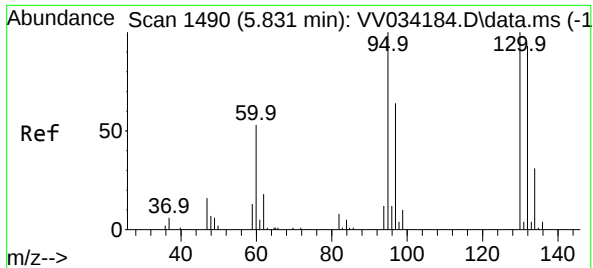

#34
 Trichloroethene
 Concen: 1.425 ug/L
 RT: 5.838 min Scan# 1492
 Delta R.T. 0.006 min
 Lab File: VV034193.D
 Acq: 15 Feb 2024 17:30

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK323

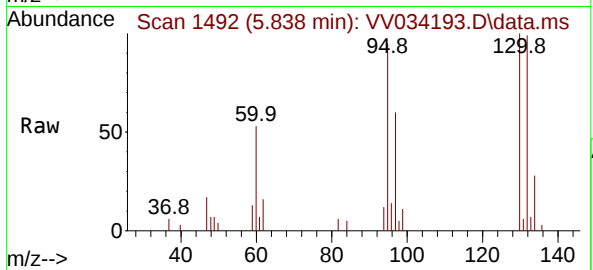

Tgt Ion:	95	Resp:	8325
Ion	Ratio	Lower	Upper
95	100		
97	63.1	45.1	83.7
132	103.6	66.0	122.6
130	104.9	72.2	134.0

