

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021524\
 Data File : VV034195.D
 Acq On : 15 Feb 2024 18:19
 Operator : SY/MD
 Sample : P1501-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E10A0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV034195.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	10	14	28	rVB2	2903	3524	1.55%	0.178%
2	1.282	67	75	90	rVB	28725	31750	13.99%	1.607%
3	1.388	102	108	117	rVB	3138	3229	1.42%	0.163%
4	1.536	146	154	165	rBV	28386	33306	14.68%	1.686%
5	2.060	306	317	330	rBV	58441	83762	36.92%	4.239%
6	3.818	854	864	906	rBV	18139	75583	33.31%	3.825%
7	4.252	983	999	1022	rBV2	40821	105012	46.29%	5.315%
8	4.960	1204	1219	1250	rBV2	90431	226876	100.00%	11.483%
9	5.535	1388	1398	1421	rBV	82853	170207	75.02%	8.615%
10	5.841	1484	1493	1515	rVB3	13077	27874	12.29%	1.411%
11	5.989	1529	1539	1568	rBV	50841	105928	46.69%	5.361%
12	6.918	1820	1828	1848	rBV2	25436	49150	21.66%	2.488%
13	7.246	1920	1930	1957	rBV	106815	188918	83.27%	9.562%
14	7.561	2020	2028	2047	rBV2	13794	27004	11.90%	1.367%
15	8.030	2165	2174	2209	rBV	99427	211853	93.38%	10.722%
16	8.786	2397	2409	2441	rBV	124449	209944	92.54%	10.626%
17	10.153	2825	2834	2855	rVB2	35589	57821	25.49%	2.926%
18	11.188	3146	3156	3178	rBV	121555	194575	85.76%	9.848%
19	11.506	3245	3255	3262	rBV3	1966	3844	1.69%	0.195%
20	11.561	3262	3272	3289	rVB	104296	165656	73.02%	8.384%




Sum of corrected areas: 1975816

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021524\
Data File : VV034195.D
Acq On : 15 Feb 2024 18:19
Operator : SY/MD
Sample : P1501-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E10A0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

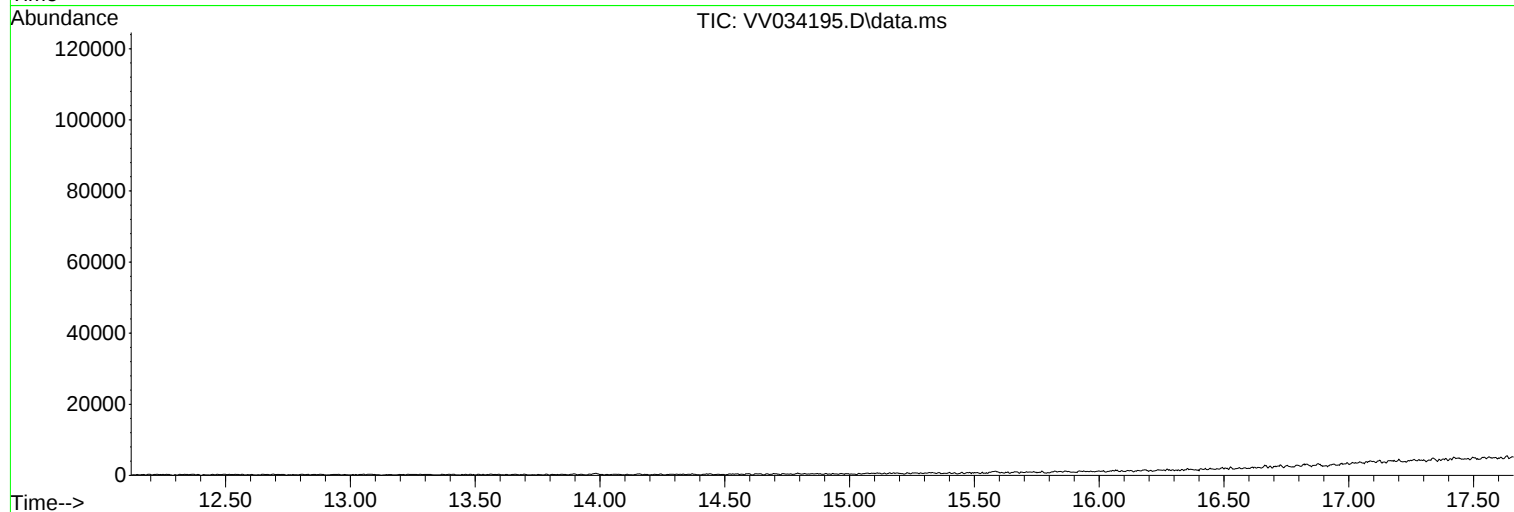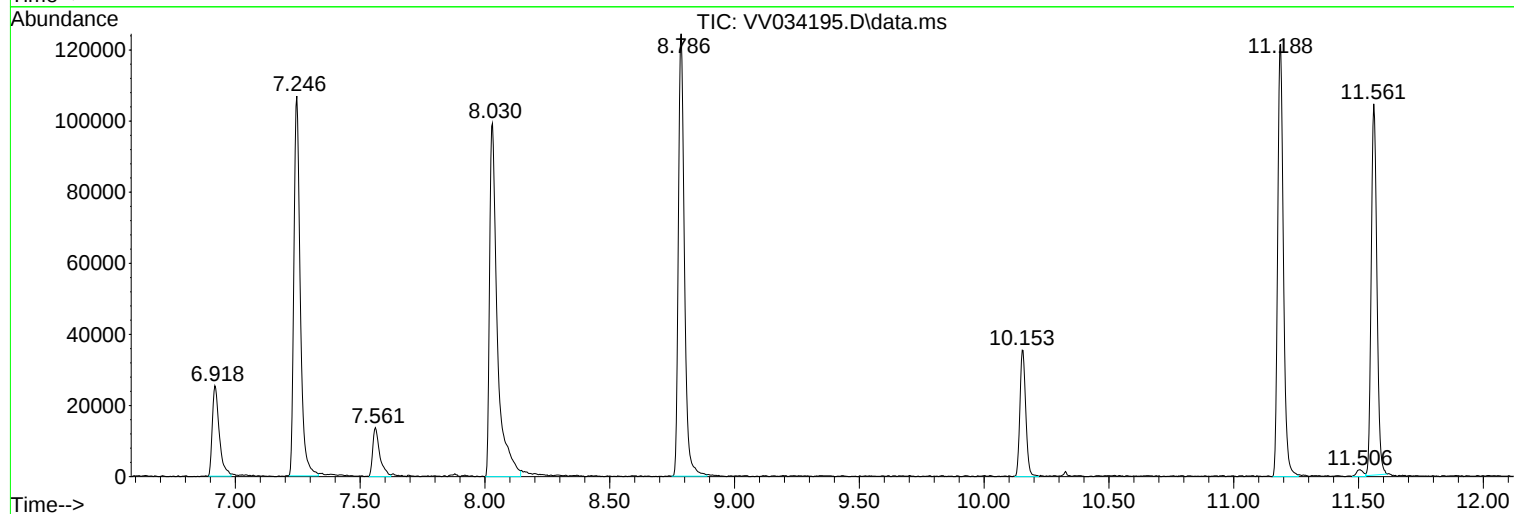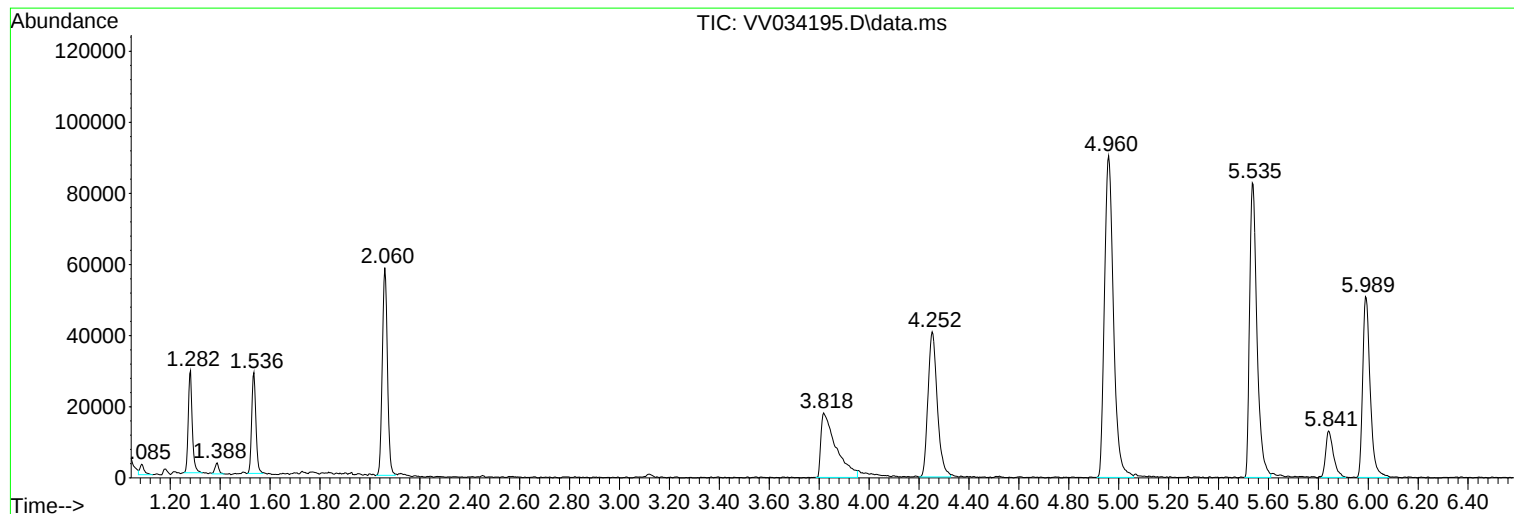

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021524\
Data File : VV034195.D
Acq On : 15 Feb 2024 18:19
Operator : SY/MD
Sample : P1501-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E10A0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021524\
Data File : VV034195.D
Acq On : 15 Feb 2024 18:19
Operator : SY/MD
Sample : P1501-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E10A0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc