

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021524\
 Data File : VV034198.D
 Acq On : 15 Feb 2024 19:33
 Operator : SY/MD
 Sample : P1501-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E10A7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV034198.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.214	50	54	62	rVB3	1867	2394	1.04%	0.123%
2	1.278	68	74	87	rVB	27720	30932	13.43%	1.584%
3	1.388	103	108	116	rVB	2106	2482	1.08%	0.127%
4	1.532	146	153	166	rVB	31168	37122	16.12%	1.901%
5	2.060	306	317	329	rVB	58103	83805	36.38%	4.291%
6	3.802	851	859	887	rBV	24715	75161	32.63%	3.849%
7	4.252	983	999	1020	rBV2	41569	106054	46.04%	5.431%
8	4.960	1205	1219	1246	rBV3	89634	230345	100.00%	11.795%
9	5.535	1388	1398	1423	rBV	78963	161612	70.16%	8.275%
10	5.844	1486	1494	1509	rBV2	6312	12587	5.46%	0.645%
11	5.989	1528	1539	1569	rBV2	51256	109395	47.49%	5.602%
12	6.918	1819	1828	1848	rBV2	24564	47858	20.78%	2.451%
13	7.246	1920	1930	1955	rBV	105573	191127	82.97%	9.787%
14	7.561	2019	2028	2050	rBV	14252	26536	11.52%	1.359%
15	7.915	2131	2138	2146	rVB4	3057	4632	2.01%	0.237%
16	8.027	2163	2173	2217	rBV	104995	213615	92.74%	10.938%
17	8.786	2399	2409	2433	rBV	119675	197586	85.78%	10.117%
18	10.156	2824	2835	2847	rBV	36421	58529	25.41%	2.997%
19	11.185	3145	3155	3177	rBV	118372	188514	81.84%	9.653%
20	11.561	3262	3272	3289	rBV	108791	172632	74.94%	8.840%




Sum of corrected areas: 1952918

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021524\
Data File : VV034198.D
Acq On : 15 Feb 2024 19:33
Operator : SY/MD
Sample : P1501-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E10A7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

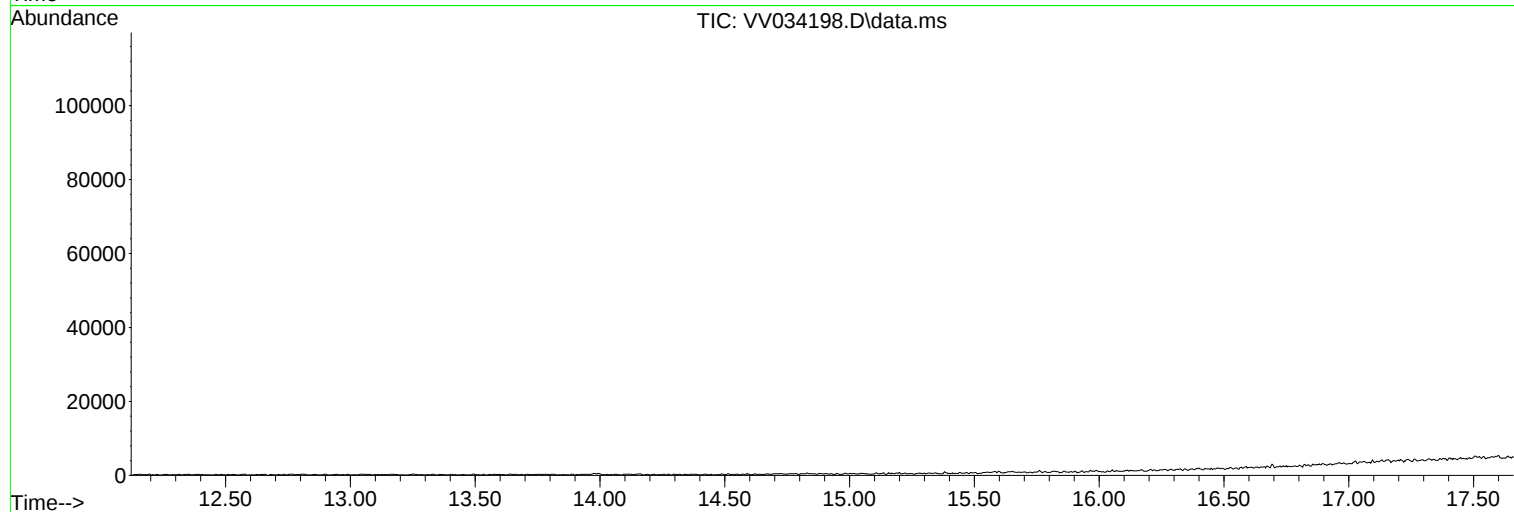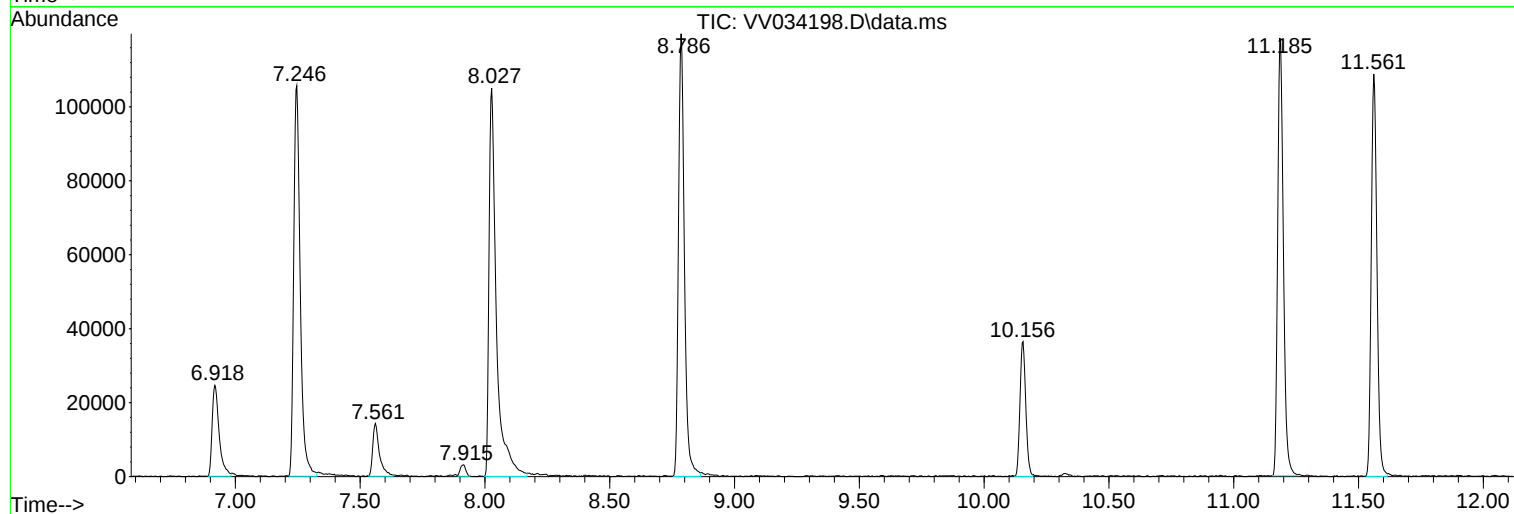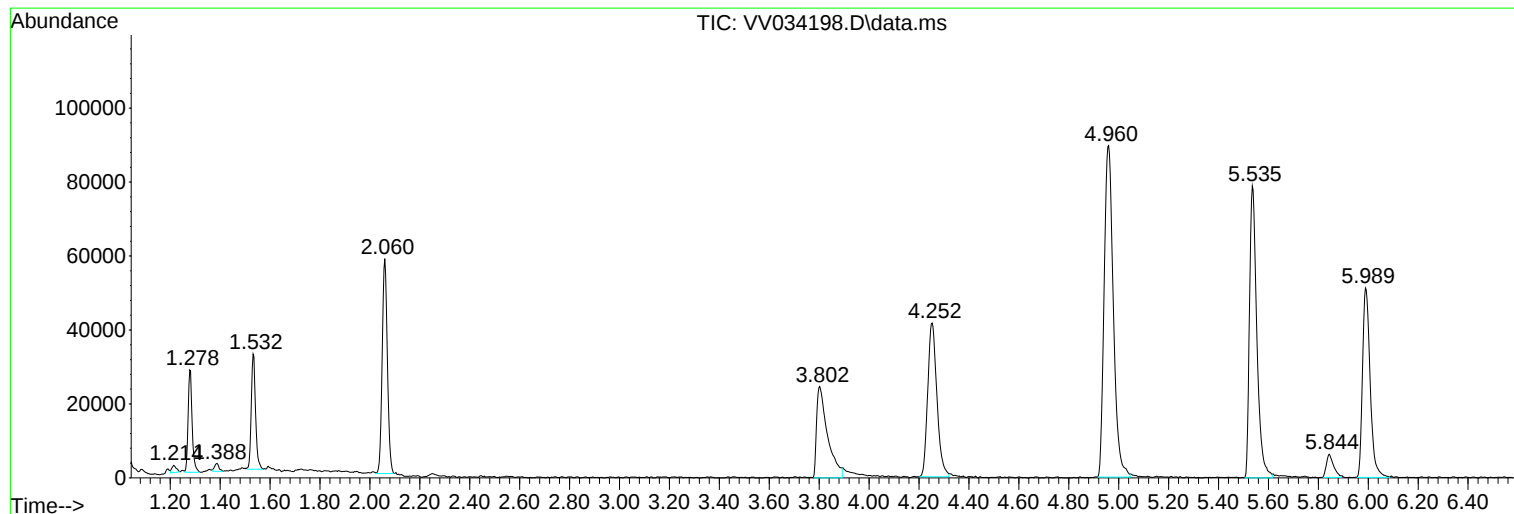

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021524\
Data File : VV034198.D
Acq On : 15 Feb 2024 19:33
Operator : SY/MD
Sample : P1501-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E10A7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021524\
Data File : VV034198.D
Acq On : 15 Feb 2024 19:33
Operator : SY/MD
Sample : P1501-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E10A7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc