

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021524\
 Data File : VV034199.D
 Acq On : 15 Feb 2024 19:58
 Operator : SY/MD
 Sample : P1501-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E10A8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV034199.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	11	14	32	rVB4	1658	2981	1.27%	0.150%
2	1.278	67	74	89	rVB	29696	30449	13.02%	1.536%
3	1.388	102	108	117	rVB	4392	4806	2.06%	0.242%
4	1.532	146	153	164	rBV	30806	36782	15.73%	1.856%
5	2.060	307	317	333	rVV	60447	86381	36.94%	4.358%
6	2.249	364	376	390	rVB3	913	2397	1.02%	0.121%
7	3.802	851	859	893	rBV	25135	81140	34.70%	4.094%
8	4.253	983	999	1026	rVB2	41925	107695	46.05%	5.434%
9	4.960	1203	1219	1245	rBV4	91651	233866	100.00%	11.799%
10	5.535	1388	1398	1424	rBV	80488	163904	70.08%	8.270%
11	5.844	1484	1494	1512	rVB6	4740	10807	4.62%	0.545%
12	5.992	1528	1540	1566	rBV2	53576	109902	46.99%	5.545%
13	6.918	1819	1828	1853	rBV	25862	49613	21.21%	2.503%
14	7.246	1919	1930	1951	rBV	109053	194480	83.16%	9.812%
15	7.561	2020	2028	2049	rBV3	13928	27265	11.66%	1.376%
16	8.027	2164	2173	2208	rBV	106525	214570	91.75%	10.826%
17	8.786	2398	2409	2431	rBV	119363	197321	84.37%	9.956%
18	10.153	2825	2834	2848	rBV	37716	59299	25.36%	2.992%
19	11.185	3142	3155	3176	rBV	121030	192476	82.30%	9.711%
20	11.561	3262	3272	3292	rBV	111658	175887	75.21%	8.874%




Sum of corrected areas: 1982021

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021524\
Data File : VV034199.D
Acq On : 15 Feb 2024 19:58
Operator : SY/MD
Sample : P1501-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E10A8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

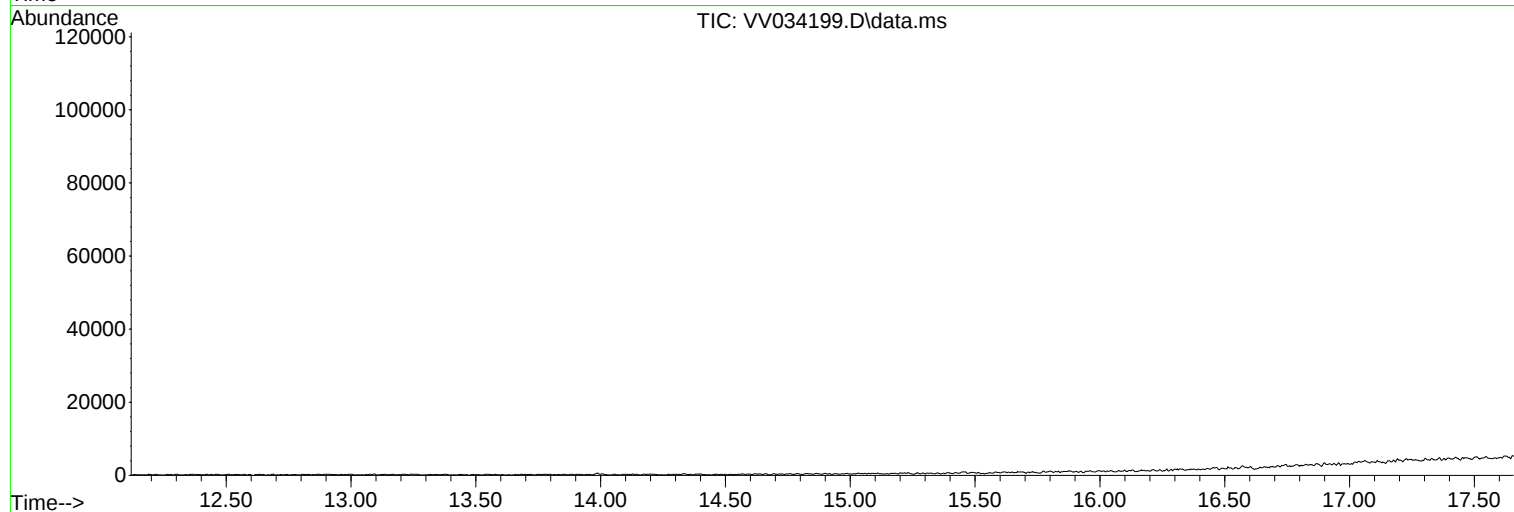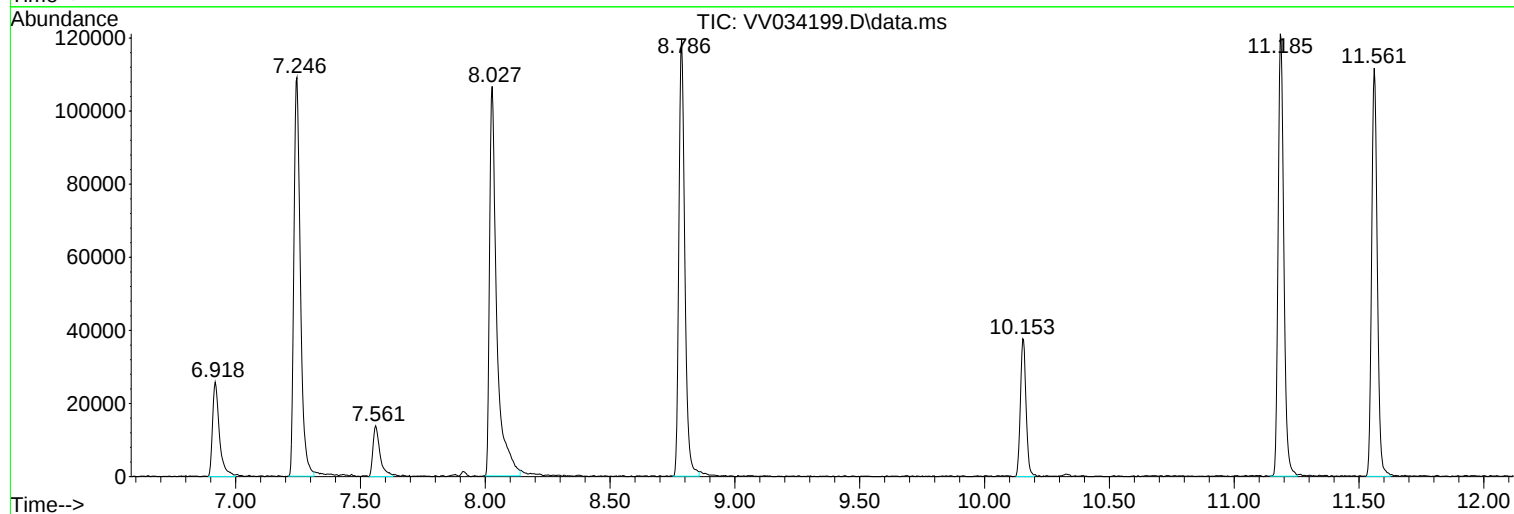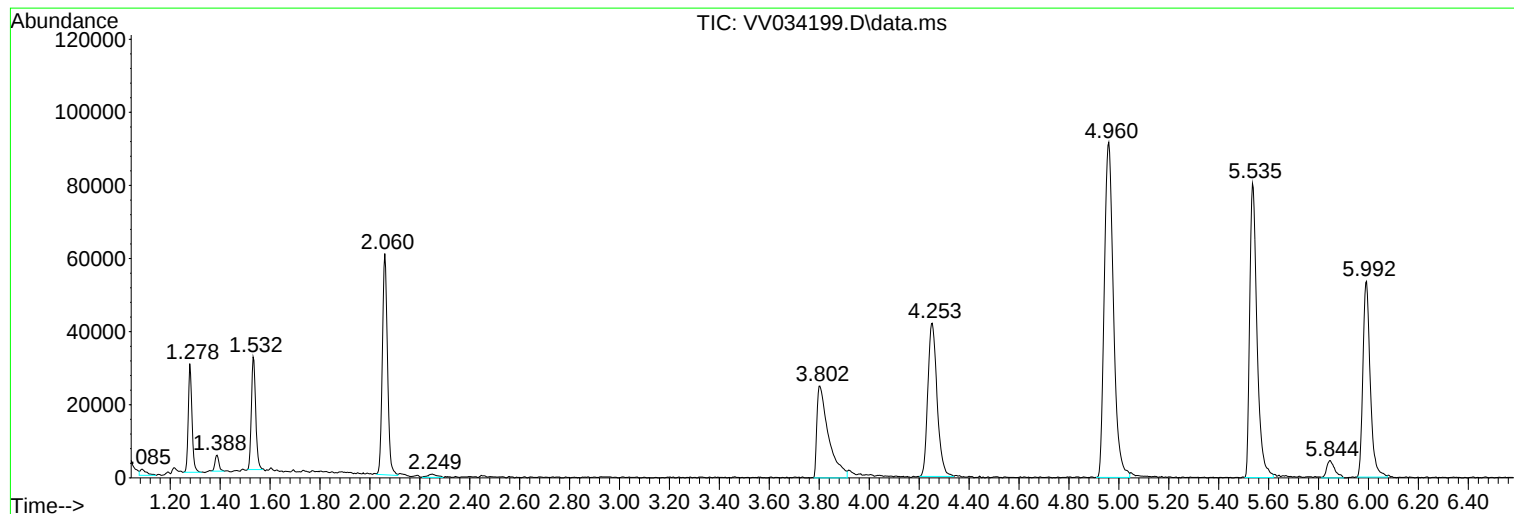

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021524\
Data File : VV034199.D
Acq On : 15 Feb 2024 19:58
Operator : SY/MD
Sample : P1501-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E10A8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021524\
Data File : VV034199.D
Acq On : 15 Feb 2024 19:58
Operator : SY/MD
Sample : P1501-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E10A8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
