
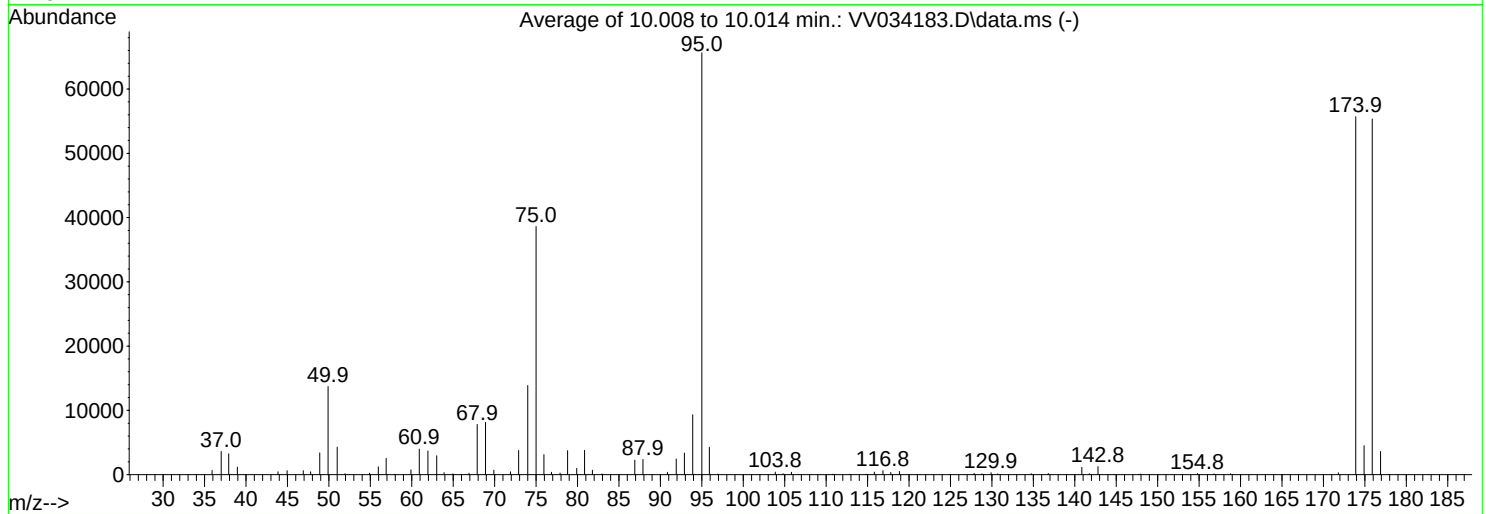


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021524\
Data File : VV034183.D
Acq On : 15 Feb 2024 11:23
Operator : SY/MD
Sample : BFB253
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB253

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Feb 20 01:47:35 2024

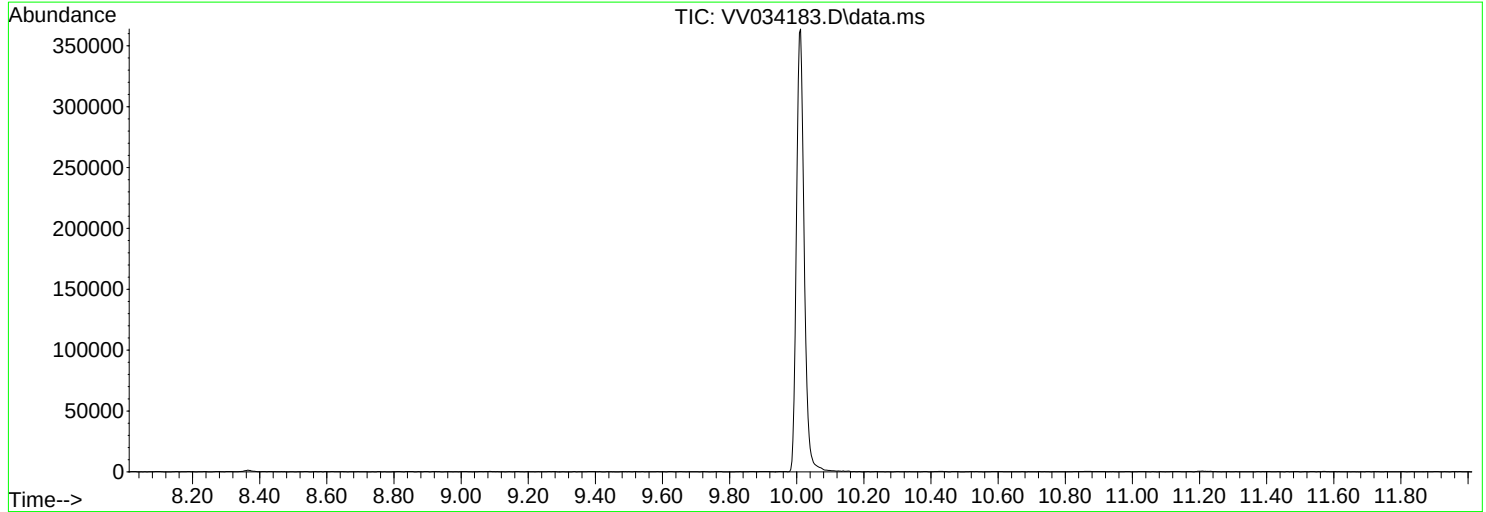

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2777

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.9	13726	PASS
75	95	30	80	58.9	38627	PASS
95	95	100	100	100.0	65629	PASS
96	95	5	9	6.5	4270	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.8	55683	PASS
175	174	5	9	8.1	4507	PASS
176	174	95	105	99.4	55341	PASS
177	176	5	10	6.5	3614	PASS

m/z	Abundance
39.80	103.0
43.80	117.0

Instrument :
MSVOA_V
ClientSampleId :
BFB253

m/z	Abundance
35.90	704.0
37.00	3773.0
37.90	3495.0
38.90	1209.0
39.90	131.0
43.90	604.0
45.00	685.0
46.90	607.0
47.80	487.0
48.90	3547.0
49.90	14485.0
51.00	4331.0
51.90	168.0
54.90	230.0
55.90	1296.0
56.90	2605.0
57.90	116.0
59.90	825.0
60.90	4173.0
61.90	3866.0
63.00	3001.0
63.90	354.0
65.00	157.0
66.90	248.0
67.90	8097.0
68.90	8403.0
69.90	788.0
71.90	495.0
72.90	3996.0
74.00	14599.0
75.00	39456.0
75.90	3313.0
76.90	414.0
77.90	239.0
78.80	3818.0
79.90	1059.0
80.80	3811.0
81.80	704.0
83.00	131.0
86.90	2397.0
87.90	2364.0
90.80	338.0
91.90	2527.0
92.90	3512.0
93.90	9405.0
95.00	67288.0
95.90	4522.0
97.00	125.0
103.90	408.0
104.80	152.0
105.80	432.0
106.70	119.0
110.80	149.0
112.90	124.0
114.80	115.0
115.80	390.0
116.80	707.0
117.80	327.0
118.90	513.0
127.80	248.0
128.80	135.0
129.90	310.0
130.70	129.0
134.80	158.0
136.80	211.0
140.80	1154.0
141.80	136.0
142.80	1190.0
147.70	143.0
154.80	165.0
156.90	146.0
158.80	140.0
171.80	286.0
173.90	55840.0
174.90	4765.0
175.90	55416.0
176.90	3655.0
177.90	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB253

m/z	Abundance
35.90	675.0
37.00	3721.0
37.90	3323.0
39.00	1191.0
39.90	128.0
43.90	578.0
44.90	621.0
46.90	656.0
47.80	451.0
48.90	3534.0
49.90	14081.0
51.00	4436.0
52.00	159.0
54.90	229.0
55.90	1238.0
56.90	2659.0
59.90	771.0
60.90	4112.0
62.00	3820.0
63.00	3038.0
63.90	360.0
65.00	126.0
66.90	252.0
67.90	8112.0
68.90	8426.0
69.90	753.0
71.90	464.0
72.90	3887.0
74.00	14259.0
75.00	39928.0
76.00	3175.0
76.90	392.0
77.90	275.0
78.80	3886.0
79.90	1018.0
80.90	3973.0
81.80	734.0
82.90	141.0
86.90	2277.0
87.90	2435.0
90.80	379.0
91.90	2537.0
92.90	3456.0
93.90	9643.0
95.00	67632.0
95.90	4437.0
96.90	112.0
103.80	409.0
104.80	156.0
105.80	400.0
110.80	112.0
112.80	106.0
114.80	101.0
115.80	406.0
116.90	639.0
117.80	352.0
118.90	497.0
127.80	217.0
128.80	135.0
129.90	310.0
130.70	131.0
134.70	156.0
136.80	201.0
140.80	1181.0
141.70	160.0
142.80	1304.0
147.90	151.0
154.80	170.0
156.80	139.0
158.80	152.0
171.80	327.0
173.90	57624.0
174.90	4651.0
175.90	57280.0
176.90	3729.0
177.90	119.0

Instrument :
MSVOA_V
ClientSampleId :
BFB253

m/z	Abundance
35.90	595.0
37.00	3322.0
37.90	2877.0
39.00	1115.0
39.90	120.0
43.90	520.0
44.90	538.0
46.90	627.0
47.80	408.0
48.90	3112.0
49.90	12612.0
51.00	4101.0
52.00	146.0
54.90	213.0
56.00	1126.0
56.90	2361.0
59.90	632.0
60.90	3651.0
62.00	3412.0
63.00	2763.0
63.90	300.0
64.90	121.0
66.90	216.0
67.90	7235.0
68.90	7598.0
69.90	581.0
71.90	407.0
72.90	3421.0
74.00	12774.0
75.00	36496.0
76.00	2868.0
76.80	342.0
77.90	259.0
78.80	3482.0
79.90	860.0
80.90	3588.0
81.80	679.0
82.90	138.0
86.90	2120.0
87.90	2271.0
90.90	382.0
91.90	2219.0
92.90	3099.0
93.90	8855.0
95.00	61968.0
95.90	3852.0
96.90	109.0
103.80	415.0
104.80	142.0
105.80	321.0
115.80	370.0
116.90	545.0
117.80	351.0
118.80	456.0
127.90	196.0
128.80	120.0
129.90	260.0
130.70	104.0
134.70	157.0
136.80	173.0
140.90	1122.0
141.70	148.0
142.80	1256.0
144.80	112.0
147.90	149.0
154.80	161.0
156.70	114.0
158.80	146.0
171.80	310.0
173.90	53584.0
174.90	4104.0
175.90	53328.0
176.90	3457.0

Instrument :
MSVOA_V
ClientSampleId :
BFB253