

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021621\
 Data File : VV020331.D
 Acq On : 16 Feb 2021 11:25
 Operator : SY/MD
 Sample : VV0216MBL01
 Misc : 5.00G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK62

Quant Time: Feb 17 00:12:48 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Feb 17 00:12:12 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	597415	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	580305	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	290631	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	236313	54.25	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 108.50%			
7) Chloroethane-d5	1.568	69	195687	54.76	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 109.52%			
11) 1,1-Dichloroethene-d2	2.108	63	338425	41.10	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 82.20%			
21) 2-Butanone-d5	3.889	46	256001	105.20	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 105.20%			
24) Chloroform-d	4.352	84	398584	51.42	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 102.84%			
26) 1,2-Dichloroethane-d4	5.037	65	273183	55.59	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 111.18%			
32) Benzene-d6	5.053	84	827347	55.03	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 110.06%			
36) 1,2-Dichloropropane-d6	6.072	67	252124	56.17	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 112.34%			
41) Toluene-d8	7.320	98	757189	53.59	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 107.18%			
43) trans-1,3-Dichloroprop...	7.625	79	114994	50.26	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 100.52%			
47) 2-Hexanone-d5	8.091	63	172787	92.53	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 92.53%			
57) 1,1,2,2-Tetrachloroeth...	10.223	84	327476	50.81	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 101.62%			
64) 1,2-Dichlorobenzene-d4	11.632	152	311414	56.63	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 113.26%			
Target Compounds					Qvalue	
25) Chloroform	4.378	83	9450	1.29	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021621\
Data File : VV020331.D
Acq On : 16 Feb 2021 11:25
Operator : SY/MD
Sample : VV0216MBL01
Misc : 5.00G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK62

Quant Time: Feb 17 00:12:48 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Feb 17 00:12:12 2021
Response via : Initial Calibration

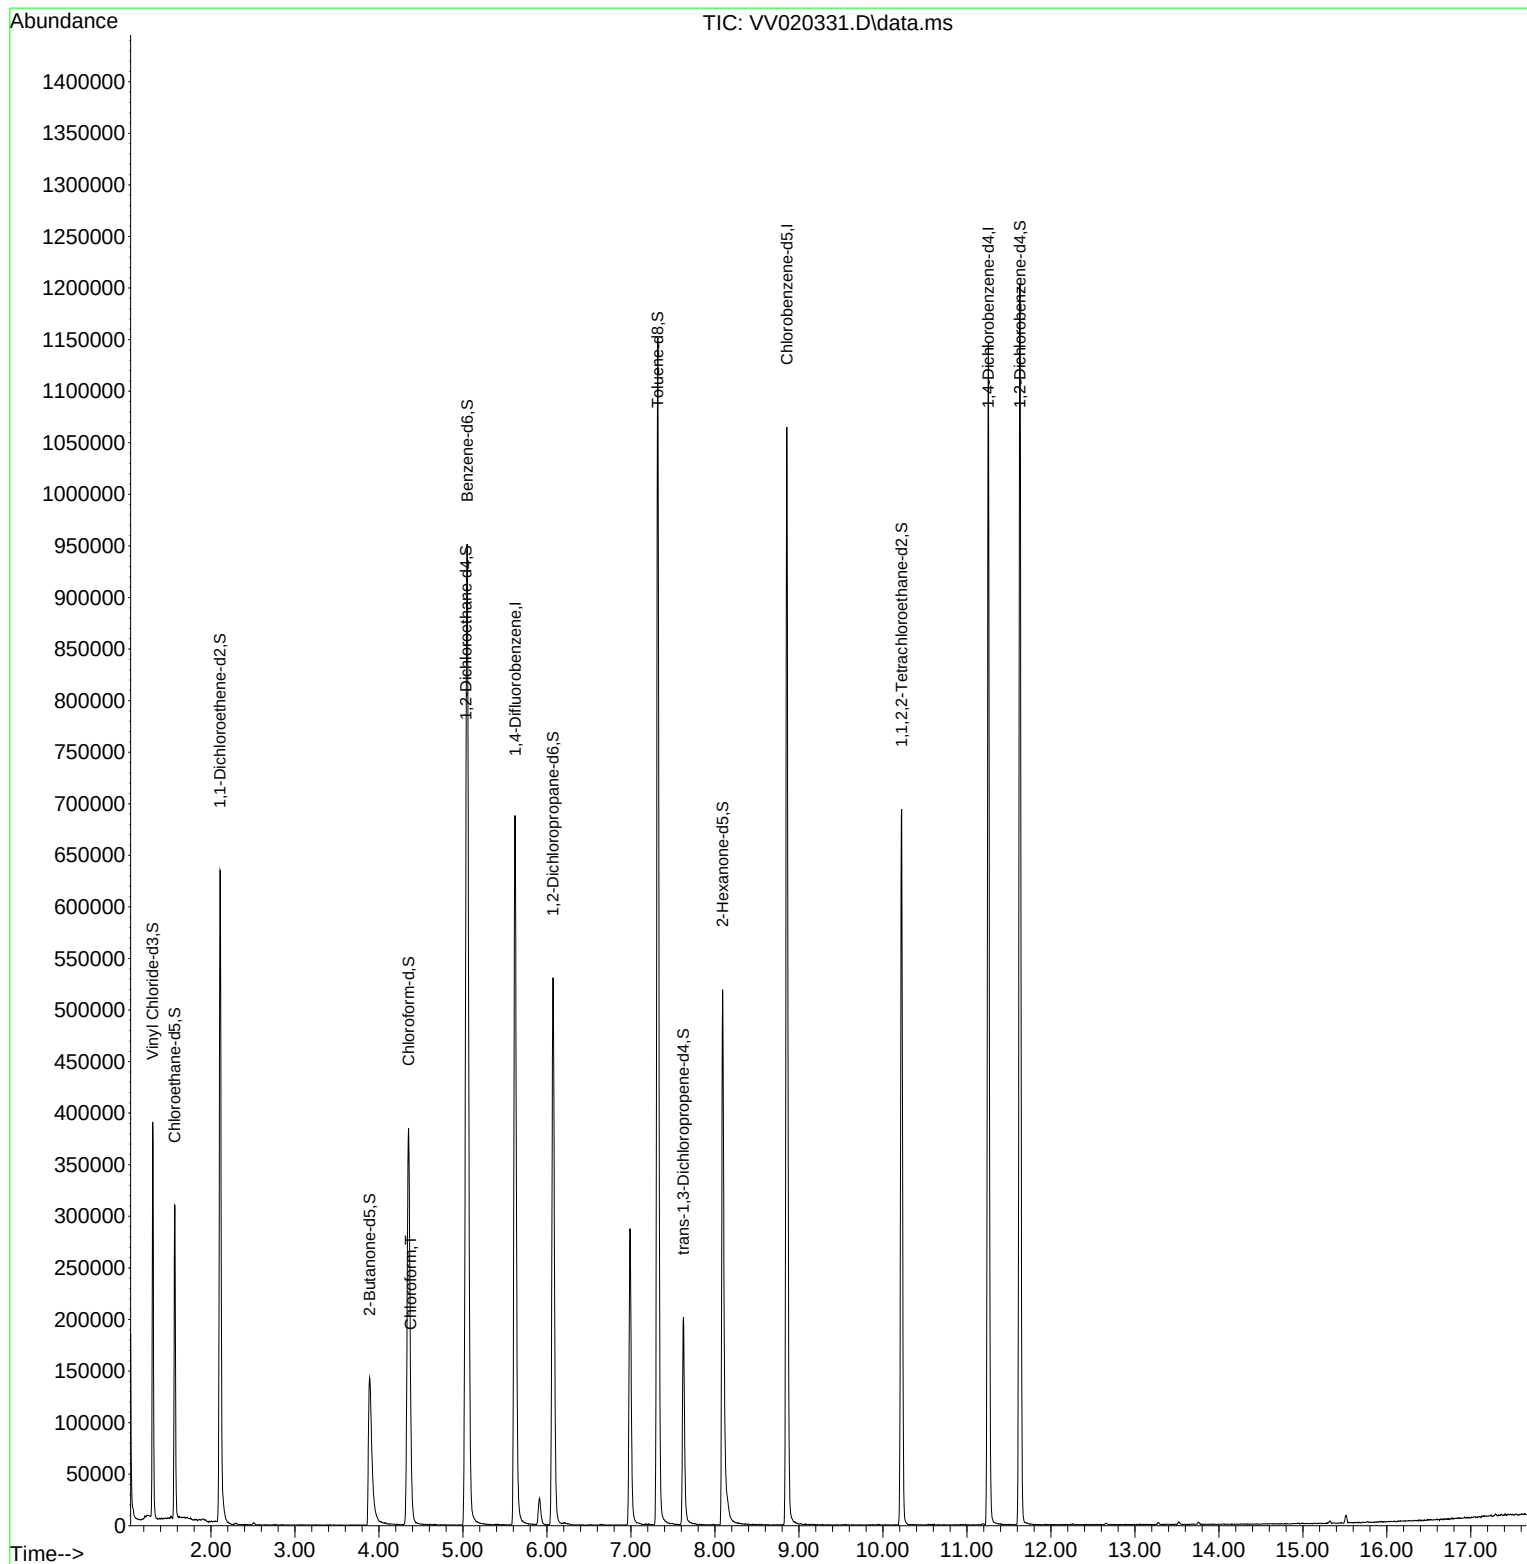

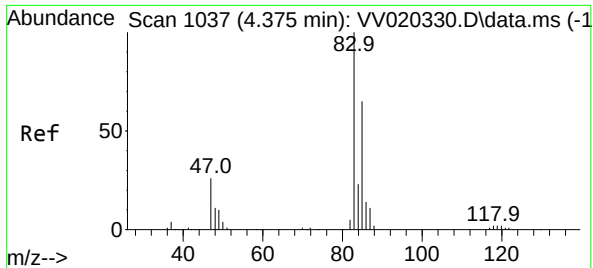

#25
Chloroform
Concen: 1.29 ug/L
RT: 4.378 min Scan# 1038
Delta R.T. 0.003 min
Lab File: VV020331.D
Acq: 16 Feb 2021 11:25

Instrument :
MSVOA_V
ClientSampleId :
VBLK62

Tgt Ion: 83 Resp: 9450
Ion Ratio Lower Upper
83 100
85 70.0 44.2 82.2

