

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021621\
 Data File : VW020334.D
 Acq On : 16 Feb 2021 13:44
 Operator : SY/MD
 Sample : VIBLK62
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK62

Quant Time: Feb 17 00:13:37 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Feb 17 00:12:12 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	559134	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	542795	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	262261	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	209114	51.30	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	102.60%
7) Chloroethane-d5	1.568	69	180556	53.98	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	107.96%
11) 1,1-Dichloroethene-d2	2.108	63	298925	38.79	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	77.58%
21) 2-Butanone-d5	3.886	46	266164	116.87	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	116.87%
24) Chloroform-d	4.352	84	380604	52.47	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	104.94%
26) 1,2-Dichloroethane-d4	5.034	65	270648	58.85	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	117.70%
32) Benzene-d6	5.053	84	777579	55.29	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	110.58%
36) 1,2-Dichloropropane-d6	6.072	67	242122	57.67	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	115.34%
41) Toluene-d8	7.320	98	696905	52.73	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	105.46%
43) trans-1,3-Dichloroprop...	7.625	79	108098	50.51	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	101.02%
47) 2-Hexanone-d5	8.092	63	173106	99.11	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	99.11%
57) 1,1,2,2-Tetrachloroeth...	10.220	84	312244	51.79	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	103.58%
64) 1,2-Dichlorobenzene-d4	11.632	152	284528	57.34	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	114.68%
Target Compounds						
25) Chloroform	4.375	83	9965	1.46	ug/L	Qvalue 83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021621\
Data File : VV020334.D
Acq On : 16 Feb 2021 13:44
Operator : SY/MD
Sample : VIBLK62
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK62

Quant Time: Feb 17 00:13:37 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Feb 17 00:12:12 2021
Response via : Initial Calibration

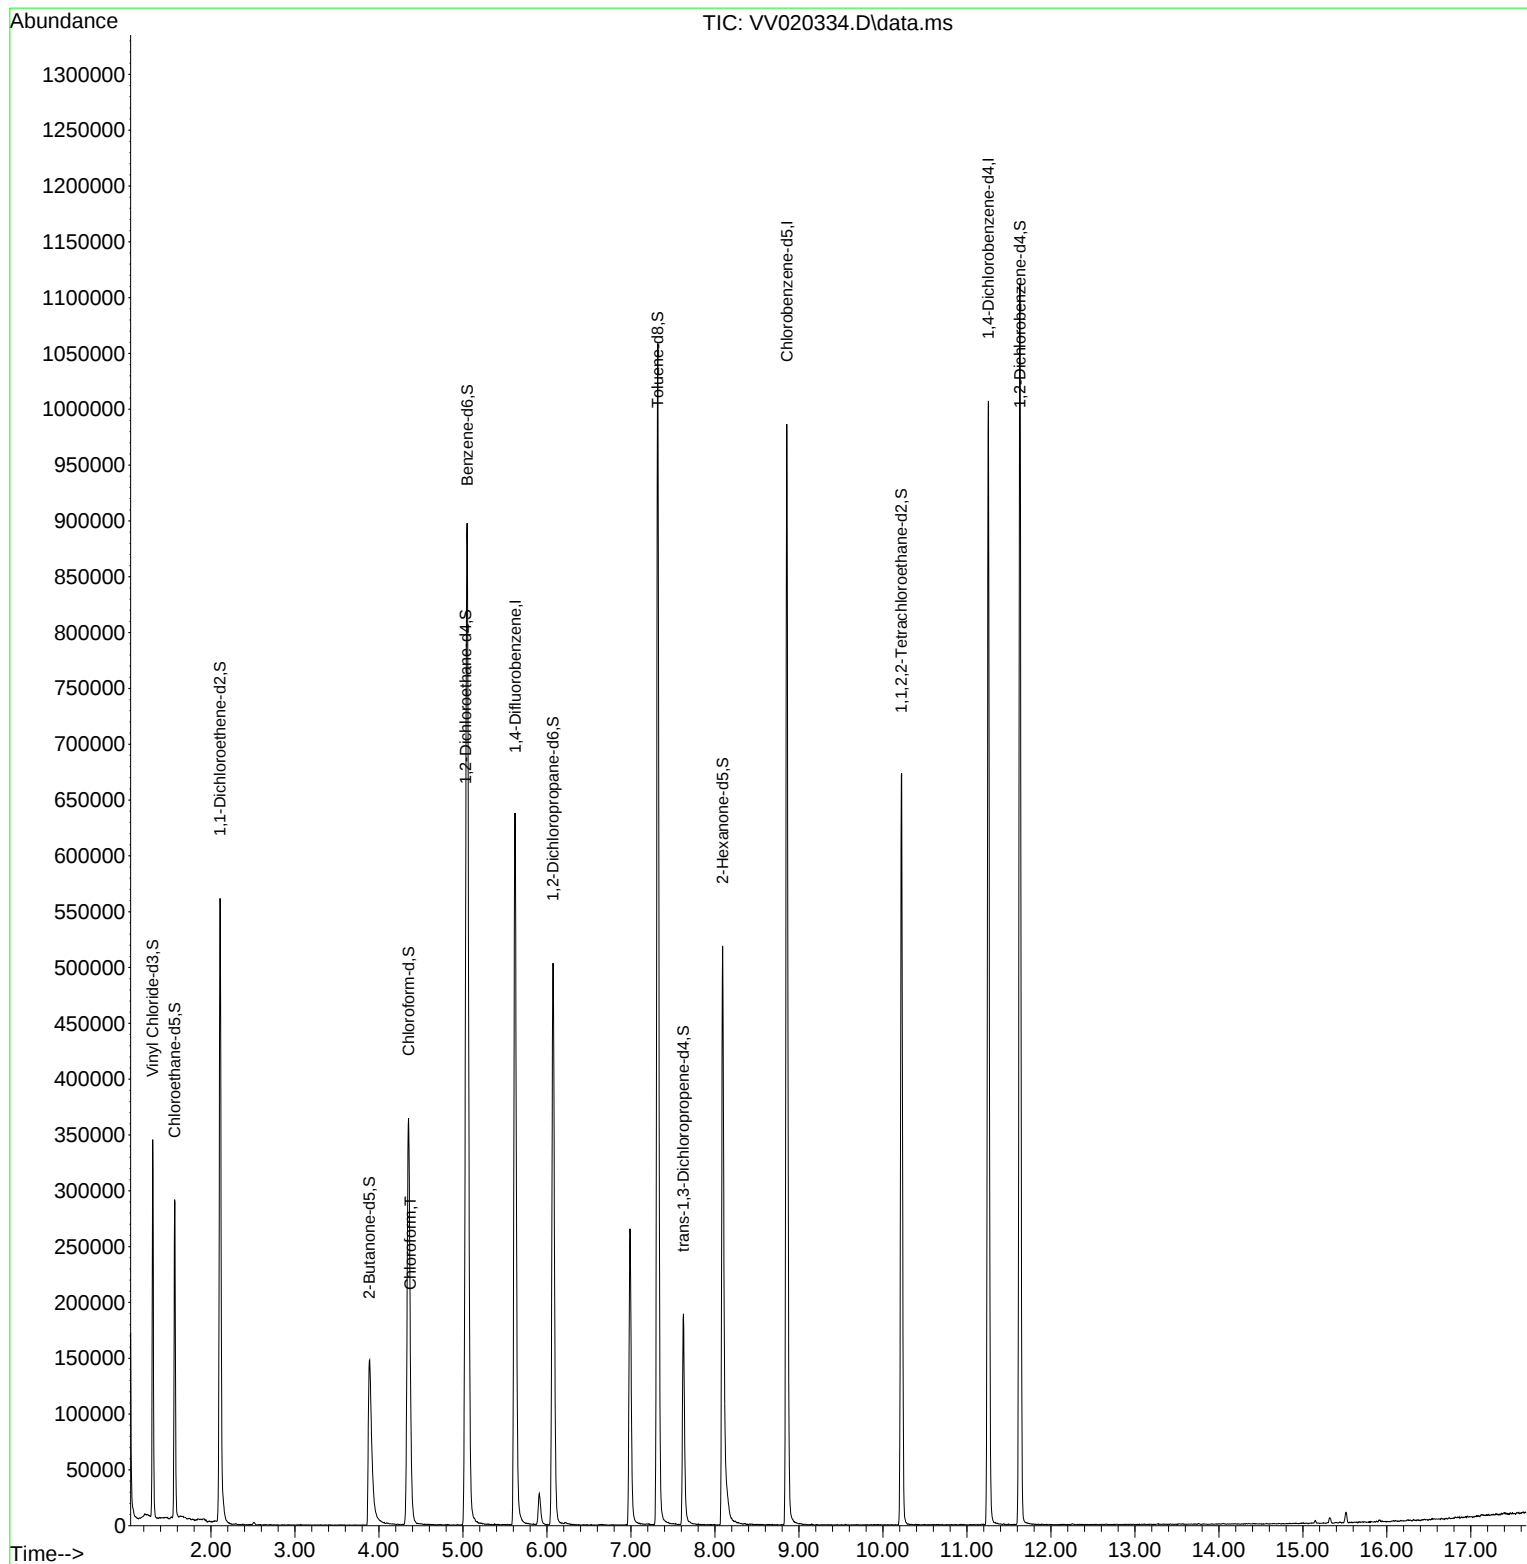

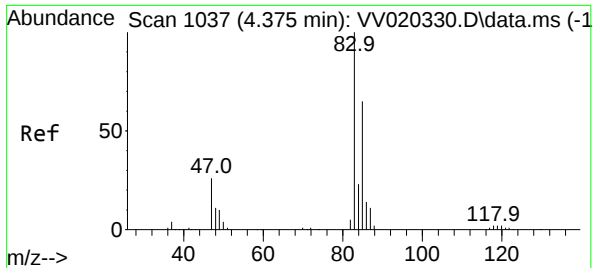

#25
Chloroform
Concen: 1.46 ug/L
RT: 4.375 min Scan# 1037
Delta R.T. 0.000 min
Lab File: VV020334.D
Acq: 16 Feb 2021 13:44

Instrument :
MSVOA_V
ClientSampleId :
VIBLK62

Tgt Ion: 83 Resp: 9965
Ion Ratio Lower Upper
83 100
85 76.6 44.2 82.2

