
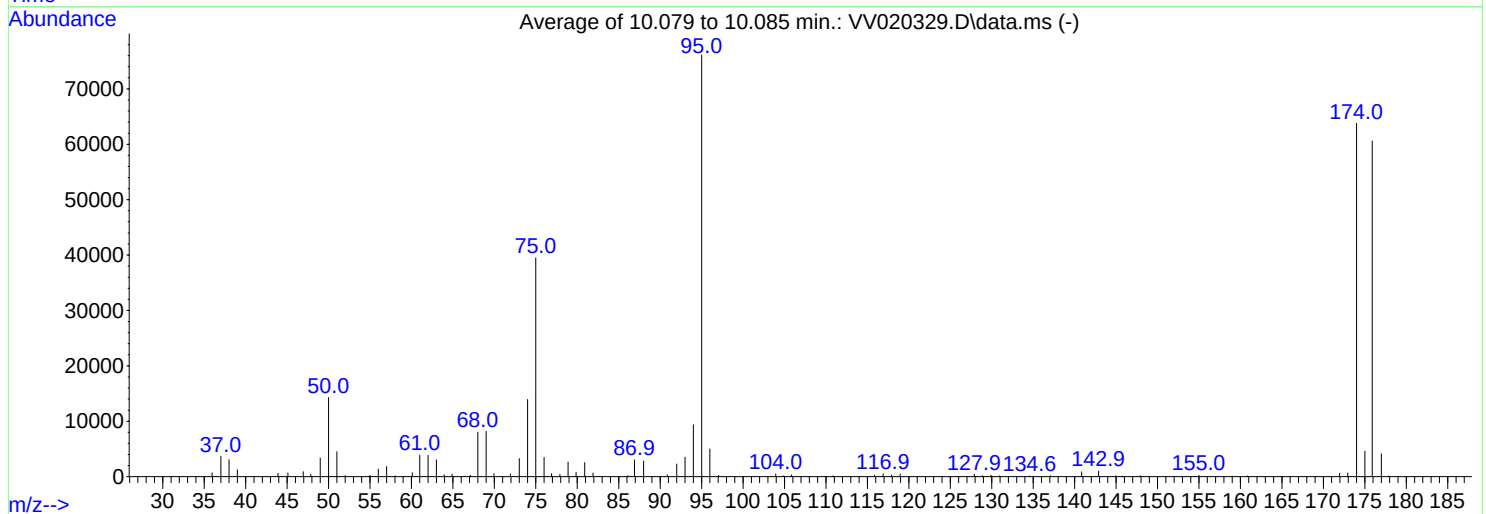


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021621\
Data File : VV020329.D
Acq On : 16 Feb 2021 09:35
Operator : SY/MD
Sample : BFB92
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB92

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Title : VOC Analysis
Last Update : Wed Feb 17 00:12:12 2021

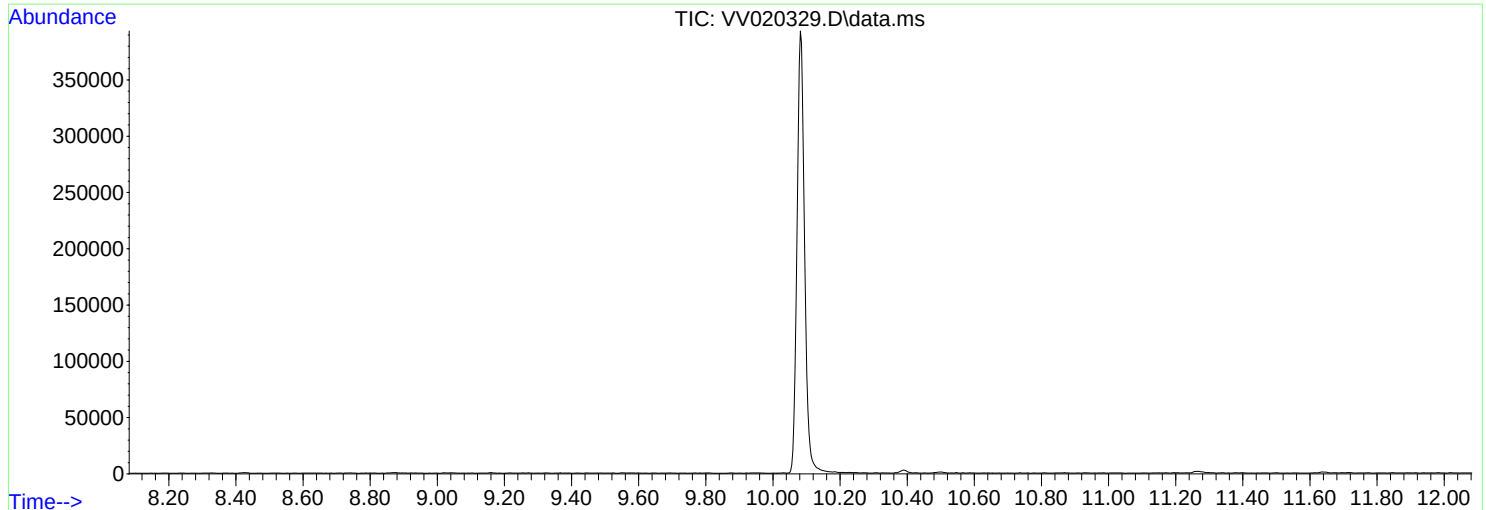

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2800

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	14266	PASS
75	95	30	80	51.9	39501	PASS
95	95	100	100	100.0	76147	PASS
96	95	5	9	6.6	5004	PASS
173	174	0.00	2	1.0	669	PASS
174	95	50	120	83.7	63773	PASS
175	174	5	9	7.2	4597	PASS
176	174	95	101	95.0	60605	PASS
177	176	5	9	6.8	4121	PASS

m/z	Abundance
35.90	628.0
37.00	3524.0
38.00	2897.0
39.00	1234.0
39.80	197.0
43.90	1051.0
45.10	632.0
46.90	946.0
47.80	366.0
49.00	3113.0
50.00	14174.0
51.00	4406.0
52.00	172.0
55.00	199.0
56.00	1271.0
57.00	1869.0
58.10	118.0
60.10	747.0
61.00	3802.0
62.00	3694.0
63.00	2907.0
63.90	309.0
64.90	458.0
67.10	190.0
68.00	7772.0
69.00	8054.0
70.00	657.0
71.90	434.0
73.00	3176.0
74.00	13692.0
75.00	37928.0
76.00	3460.0
76.90	573.0
77.90	313.0
78.90	2654.0
79.80	771.0
80.90	2462.0
81.90	617.0
86.10	202.0
86.90	3264.0
88.00	2916.0
90.90	368.0
92.00	2213.0
93.00	3212.0
94.00	9315.0
95.00	73288.0
96.00	4936.0
97.10	244.0
103.90	470.0
104.90	175.0
105.90	319.0
110.90	142.0
115.90	232.0
116.90	458.0
117.80	318.0
119.00	493.0
127.90	364.0
128.90	203.0
130.00	304.0
130.90	149.0
134.60	115.0
137.10	194.0
140.90	852.0
142.90	986.0
144.00	112.0
144.90	151.0
147.80	154.0
155.00	220.0
159.00	115.0
160.80	131.0
170.70	116.0
171.90	621.0
172.90	648.0
174.00	59816.0
175.00	4323.0
175.90	56192.0
177.00	3954.0
177.90	134.0

Instrument :
MSVOA_V
ClientSampleId :
BFB92

m/z	Abundance
36.00	683.0
37.00	3859.0
38.00	3179.0
39.00	1272.0
39.90	220.0
43.90	1055.0
45.10	709.0
47.00	949.0
47.80	402.0
49.00	3473.0
50.00	14713.0
51.00	4691.0
52.00	206.0
55.00	190.0
56.00	1404.0
57.00	1863.0
58.00	145.0
60.10	759.0
61.00	4042.0
62.00	4023.0
63.00	3149.0
63.90	350.0
64.90	496.0
66.90	196.0
67.10	200.0
68.00	8354.0
69.00	8461.0
70.00	559.0
72.00	520.0
73.00	3348.0
74.00	14477.0
75.00	40968.0
76.00	3611.0
76.90	590.0
77.90	424.0
78.90	2743.0
79.90	848.0
80.90	2611.0
81.90	703.0
86.10	196.0
86.90	3124.0
88.00	2883.0
90.90	366.0
92.00	2344.0
93.00	3737.0
94.00	9797.0
95.00	78760.0
96.00	5175.0
97.10	226.0
103.90	519.0
104.90	141.0
105.80	334.0
110.90	166.0
115.80	273.0
116.90	532.0
117.90	297.0
119.00	521.0
127.90	414.0
128.80	160.0
129.90	291.0
130.90	162.0
134.60	138.0
135.00	124.0
137.10	197.0
140.90	921.0
142.90	1036.0
145.00	181.0
145.70	118.0
147.90	184.0
152.90	107.0
155.00	267.0
159.00	135.0
160.80	156.0
172.00	635.0
172.90	678.0
174.00	65896.0
175.00	4718.0
175.90	62680.0
177.00	4311.0
177.90	154.0

Instrument :
MSVOA_V
ClientSampleId :
BFB92

m/z	Abundance
36.00	751.0
37.00	3628.0
38.00	3095.0
39.00	1267.0
39.90	234.0
44.00	1040.0
45.10	647.0
47.00	822.0
47.90	416.0
49.00	3473.0
50.00	13912.0
51.00	4403.0
52.00	200.0
55.00	196.0
56.00	1390.0
57.00	1721.0
58.00	150.0
60.10	682.0
61.00	3818.0
62.00	3855.0
63.00	3061.0
64.00	352.0
64.90	460.0
67.20	230.0
68.00	7940.0
69.00	8041.0
69.90	483.0
72.00	525.0
73.00	3255.0
74.00	13566.0
75.00	39608.0
76.00	3357.0
76.90	515.0
77.90	489.0
78.90	2493.0
79.90	849.0
80.90	2542.0
81.90	643.0
86.10	140.0
86.90	2708.0
88.00	2709.0
90.80	329.0
92.00	2269.0
93.00	3652.0
94.00	8979.0
95.00	76392.0
96.00	4901.0
97.00	190.0
104.00	462.0
104.80	129.0
105.80	337.0
110.80	149.0
115.20	100.0
115.90	270.0
116.90	581.0
118.00	304.0
118.90	490.0
127.90	417.0
128.90	124.0
129.80	289.0
130.90	150.0
134.60	132.0
135.10	146.0
137.10	161.0
140.80	862.0
142.90	927.0
144.90	206.0
145.80	131.0
148.00	218.0
155.00	272.0
157.10	107.0
159.00	116.0
160.80	154.0
172.00	563.0
173.00	680.0
174.00	65608.0
175.00	4749.0
175.90	62944.0
177.00	4099.0
177.90	158.0

Instrument :
MSVOA_V
ClientSampleId :
BFB92

m/z	Abundance
39.90	219.0
43.90	451.0

Instrument :
MSVOA_V
ClientSampleId :
BFB92