

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021623\
 Data File : VV030057.D
 Acq On : 16 Feb 2023 10:26
 Operator : SY/MD
 Sample : VV0216WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK209

Quant Time: Feb 17 00:58:09 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM021523.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Feb 16 01:49:02 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	13204	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	12413	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	7562	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	4852	0.363	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	72.000%		
4) 1,2-Dichloroethane-d4	4.945	65	3893	0.541	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	108.000%		
7) 1,2-Dichloropropane-d6	5.995	67	4424	0.476	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	96.000%		
8) Toluene-d8	7.253	98	14448	0.505	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	102.000%		
10) 1,1,2,2-Tetrachloroeth...	10.146	84	3472	0.508	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	102.000%		
Target Compounds						
6) Trichloroethene	5.852	95	135	0.014	ug/L	Qvalue # 88

(#) = qualifier out of range (m) = manual integration (+) = signals summed




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021623\
Data File : VV030057.D
Acq On : 16 Feb 2023 10:26
Operator : SY/MD
Sample : VV0216WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK209

Quant Time: Feb 17 00:58:09 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM021523.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Feb 16 01:49:02 2023
Response via : Initial Calibration

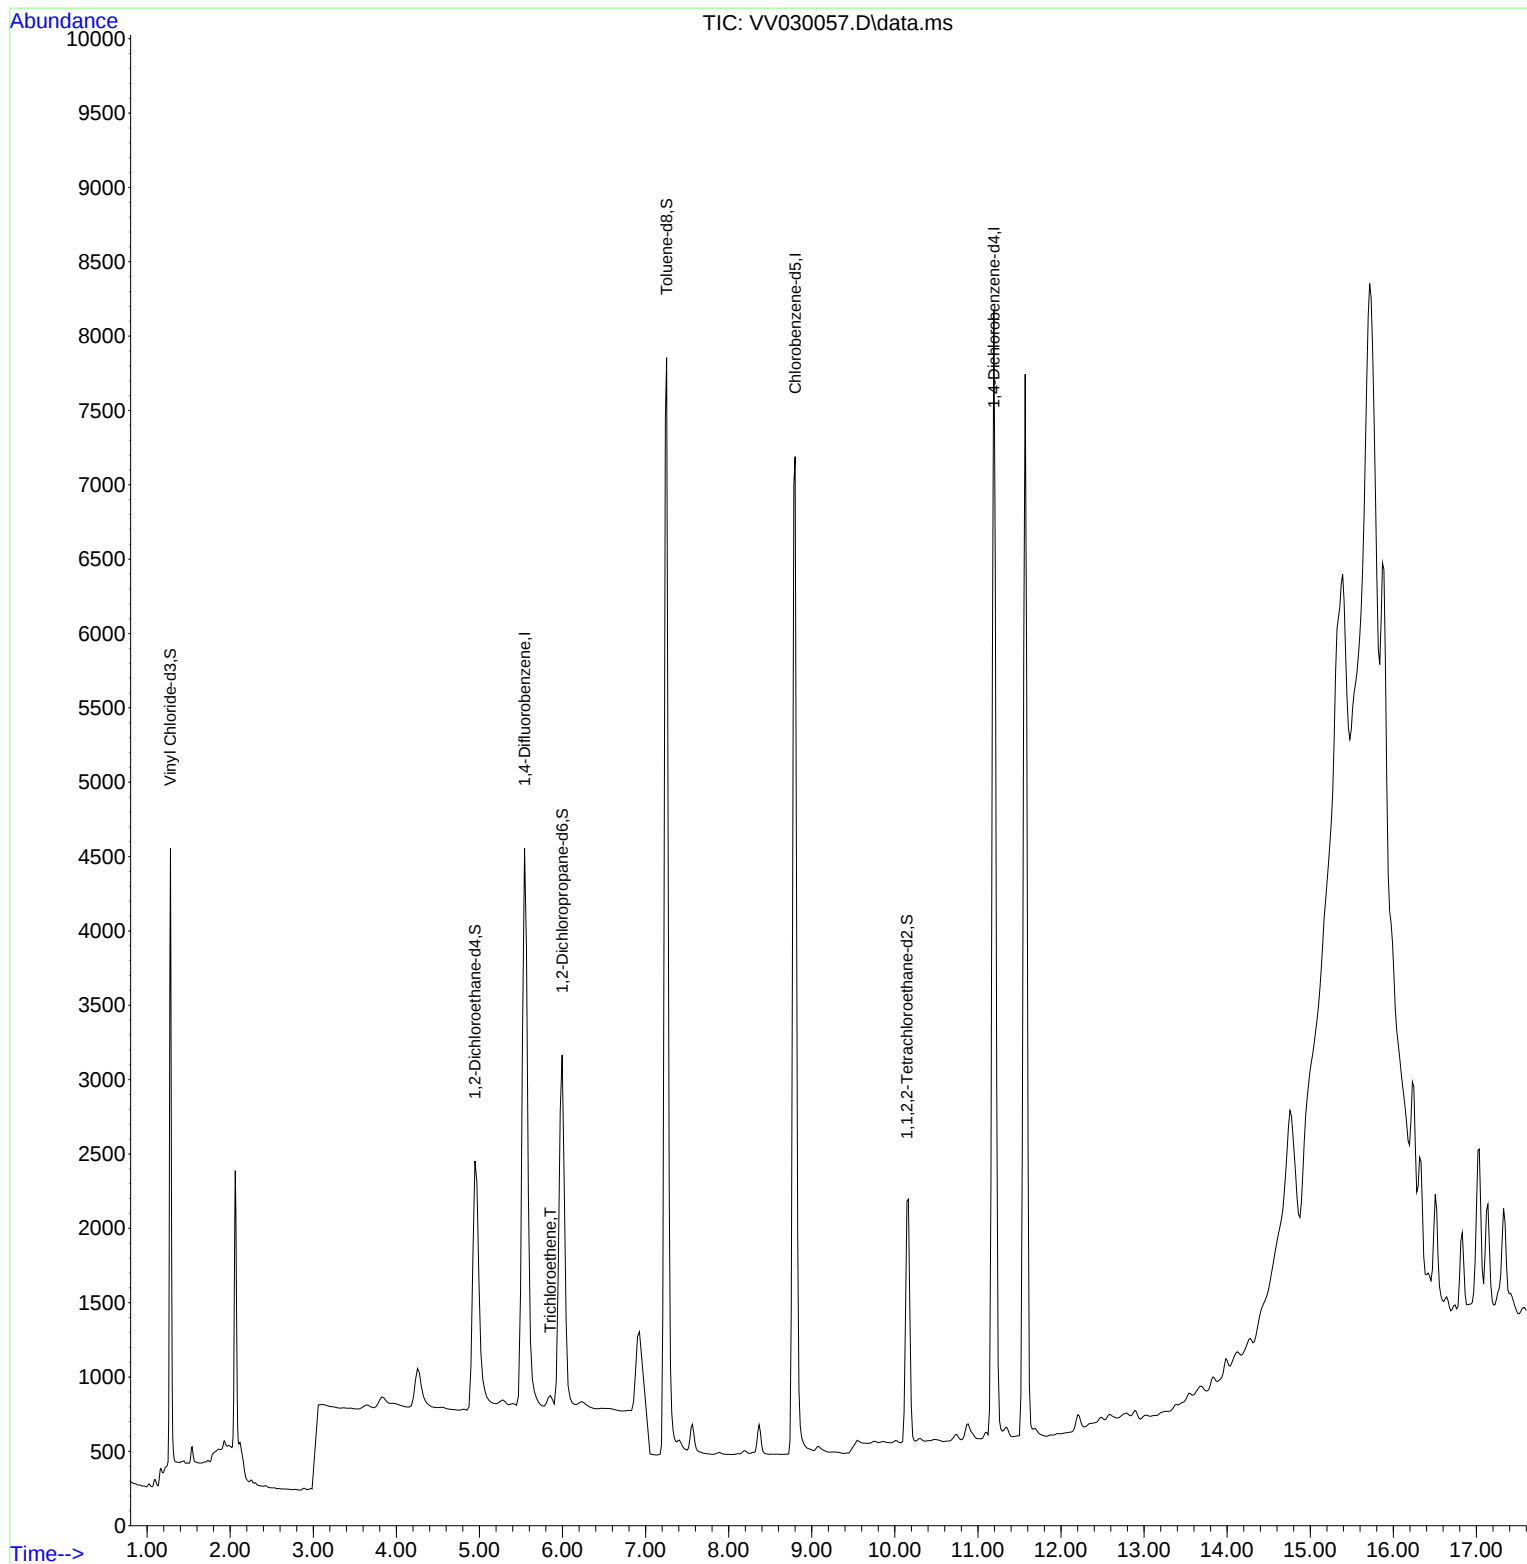

Abundance Scan 428 (5.828 min): VV030056.D\data.ms (-42

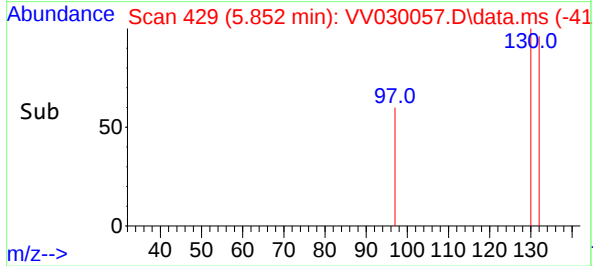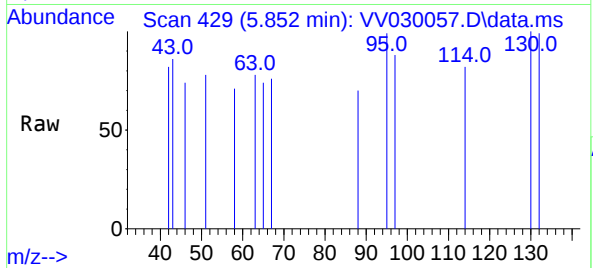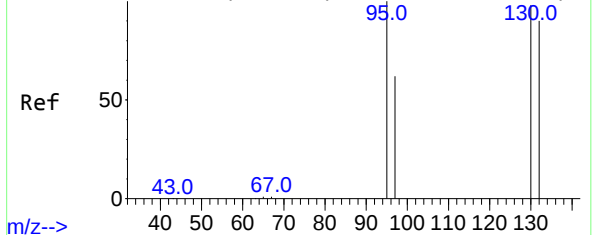

#6
Trichloroethene
Concen: 0.014 ug/L
RT: 5.852 min Scan# 41
Delta R.T. -0.000 min
Lab File: VV030057.D
Acq: 16 Feb 2023 10:26

Instrument :
MSVOA_V
ClientSampleId :
VBLK209

Tgt Ion: 95	Resp:	135
Ion	Ratio	Lower Upper
95	100	
97	89.3	46.9 87.1#
132	100.0	74.9 139.1
130	101.3	76.6 142.2

